INSTALLATION REPORT

DataMaster DMT:	103509
Location:	Hardwick-Greensboro PD
Calibration Date:	09/21/2011
Certification Date:	09/21/2011
Installation Date:	01/04/2013
Installed by:	ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 44.1°C
Digital Sim    = 33.8°C

SETTINGS
Lamp Voltage   = 1.58 V
Cooler Voltage = 1.54 V
Bias Voltage   = 81 V
Chopper Freq   = 533 Hz

PUMP INFO
Flow Rate = 6.226 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3305    0.3327
MIN(V)   0.3287    0.3309

FILTER INFO
Filter 1   0.332  Zero = true
Filter 2   0.645  Zero = true
Filter 3   0.264  Zero = true

CALIBRATION CHECK
Xq  = 0.081  2.40%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Average	= 0.102 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

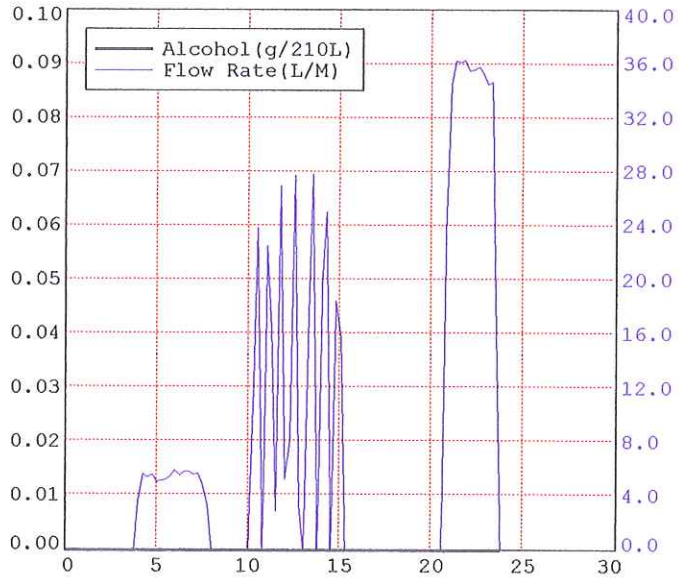

INSTALLATION PASSED

Performed by _____ Date 01/04/2013

Reviewed by _____ Date 1/7/2013