ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 103509
Location: Hardwick-Greensboro PD
Calibration Date: 09/21/2011
Certification Date: 09/21/2011
Installation Date: 01/04/2013
RPC Date: 06/14/2013
Supervisor Name: MICHAEL R GERO

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube    = 45.6°C
Digital Sim    = 33.8°C

SETTINGS
Lamp Voltage   = 1.58 V
Cooler Voltage = 1.54 V
Bias Voltage   = 81 V
Chopper Freq   = 540 Hz

PUMP INFO
Flow Rate = 6.153 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3376    0.3400
MIN(V)   0.3360    0.3380

FILTER INFO
Filter 1   0.338   Zero = true
Filter 2   0.656   Zero = true
Filter 3   0.288   Zero = true

CALIBRATION CHECK
Xq  = 0.082  2.62%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 12-84-100
Range	= 0.096 - 0.106
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

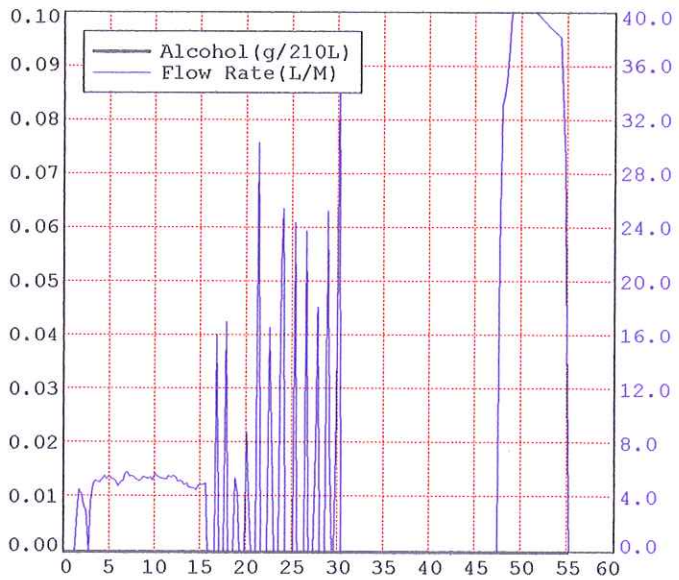

Performed by _____ Date 06/14/2013

Reviewed by _____ Date 6/24/13

6/24/2013