ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 104409
Location: Winooski PD
Calibration Date: 12/19/2011
Certification Date: 12/20/2011
Installation Date: 12/23/2011
RPC Date: 02/05/2013
Supervisor Name: JASON R NOKES

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.72 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 537 Hz

PUMP INFO
Flow Rate = 6.162 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.2177	0.2199
MIN(V)	0.2163	0.2183

FILTER INFO
Filter 1 0.219 Zero = true
Filter 2 0.449 Zero = true
Filter 3 0.612 Zero = true

CALIBRATION CHECK
Xq = 0.081 1.09%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration = 0.098 g/210L
Lot # = 12-88-100
Range = 0.093 - 0.103
Average = 0.098 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

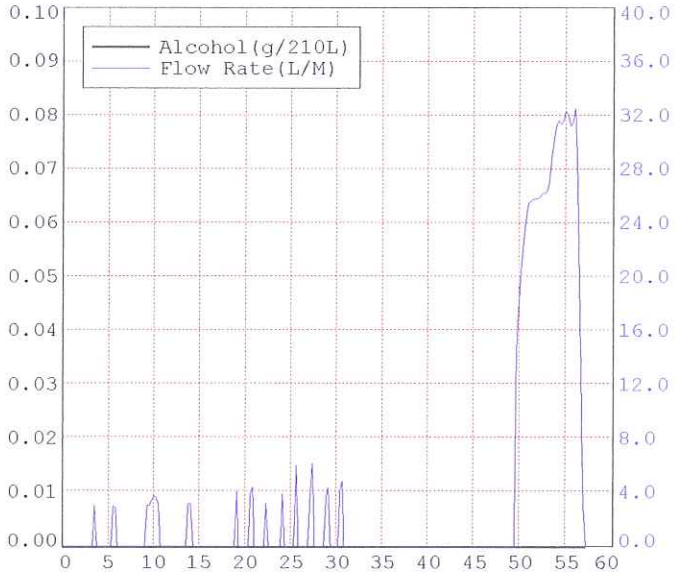

Performed by Jason R Nokes 914 Date 02/05/2013 2/11/2013

Reviewed by [signature] Date 2/8/13

Status Record History

Status Date	Status Time	Test Type	Status Message
01/30/2013	02:20:50	DUI Subject Record	Simulator Out of Range

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
01/30/2013	02:19:13	sbpd	D BRUNELLE			0.093		Simulator Out of Range

3-DB

DATAMASTER DMT MAINTENANCE LOG

Winooski Police
Department/Agency

104409
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/5/13	[For RF **DataMaster Simulator Solution** Lot # 12-88-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 11/9/2012 Expires: 11/9/2013 OPENED: ace Label Here]	Nokes 914
2/5/13	RPC	Nokes 914
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011

4 AB