INSTALLATION REPORT

DataMaster DMT: 104609
Location: UVM PD
Calibration Date: 07/31/2014
Certification Date: 07/31/2014
Installation Date: 07/31/2014
Installed by: AMANDA BOLDUC

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube = 46.7°C
Digital Sim = 33.9°C

SETTINGS
Lamp Voltage = 1.75 V
Cooler Voltage = 1.80 V
Bias Voltage = 81 V
Chopper Freq = 536 Hz

PUMP INFO
Flow Rate = 6.315 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.2364	0.2402
MIN(V)	0.2350	0.2388

FILTER INFO
Filter 1 0.239 Zero = true
Filter 2 0.555 Zero = true
Filter 3 0.216 Zero = true

CALIBRATION CHECK
Xq = 0.079 0.55%

Accuracy and Precision Check

Concentration = 0.098 g/210L
Lot # = 14-05-100
Range = 0.093 - 0.103
Average = 0.096 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

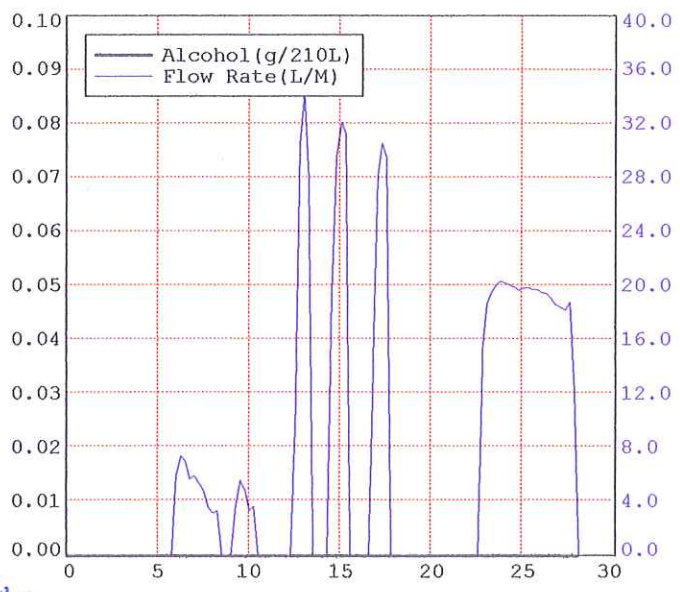

INSTALLATION PASSED

Thermometer S/N 111814517 33.9°C 8/4/14

Performed by A Bold 8/4/14 **Date** 07/31/2014

Reviewed by [signature] **Date** 8/5/2014