INSTALLATION REPORT

DataMaster DMT: 122306
Location: Essex County So
Calibration Date: 08/30/2011
Certification Date: 08/30/2011
Installation Date: 06/26/2012
Installed by: TRISHA L CONTI

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.5°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.68 V
Cooler Voltage = 1.72 V
Bias Voltage   = 80 V
Chopper Freq   = 541 Hz

PUMP INFO
Flow Rate = 4.349 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0522    0.0549
MIN(V)   0.0506    0.0533

FILTER INFO
Filter 1   0.054  Zero = true
Filter 2   0.363  Zero = true
Filter 3   0.796  Zero = true

CALIBRATION CHECK
Xq  = 0.098  0.18%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-77-100
Range	= 0.094 - 0.104
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

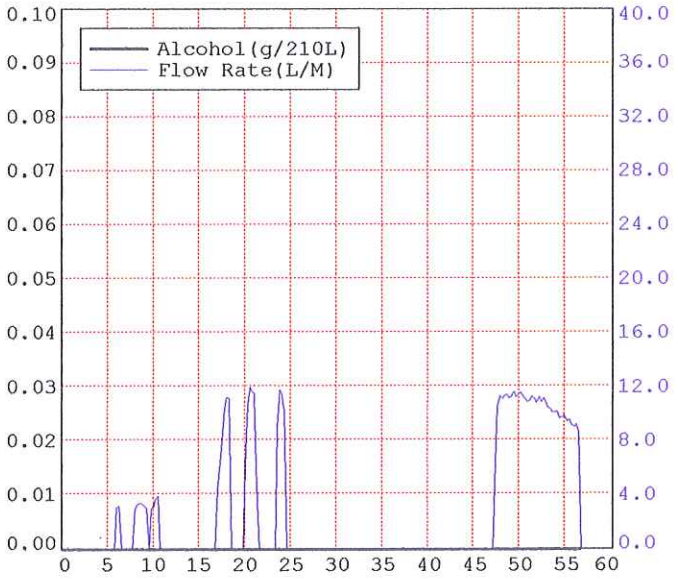

INSTALLATION PASSED

Performed by TLCA **Date** 06/26/2012

Reviewed by [signature] **Date** 6/28/12

TLCA 6/28/2012