INSTALLATION REPORT

DataMaster DMT: 100171
Location: St. Albans VSP
Calibration Date: 01/25/2012
Certification Date: 01/26/2012
Installation Date: 01/27/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 46.6°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.75 V
Cooler Voltage = 1.71 V
Bias Voltage   = 81 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 5.411 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0659   -0.0644
MIN(V)   -0.0701   -0.0679

FILTER INFO
Filter 1  -0.064  Zero = true
Filter 2   0.156  Zero = true
Filter 3   0.960  Zero = true

CALIBRATION CHECK
Xq  = 0.080  2.12%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-51-100
Range	= 0.095 - 0.105
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

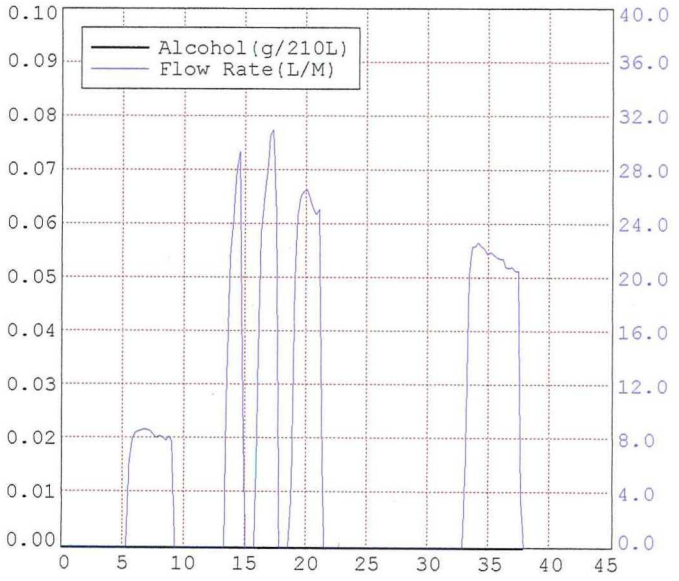

INSTALLATION PASSED

Performed by _____ Date 01/27/2012

Reviewed by _____ Date 1-27-12

Reviewed 01/30/12