

ROUTINE PERFORMANCE CHECK REPORT

RECEIVED

DEC 05 2011

DataMaster DMT: 103206
 Location: ST. ALBANS PD
 Calibration Date: 03/18/2011
 Certification Date: 03/18/2011
 Installation Date: 03/18/2011
 RPC Date: 11/18/2011
 Supervisor Name: HOLLY B MOORE



VERMONT
Vermont Department of Health Laboratory

DEPARTMENT OF HEALTH

Diagnostic Results

VERSIONS
 DMT 1.05
 PIC 2.06
 Modem 1.06
 Questions 1.00
 Reports 1.02

TEMPERATURES
 Sample Chamber = 49.15°C
 Breath Tube = 47.64°C
 Digital Sim = 33.9°C

SETTINGS
 Lamp Voltage = 1.90 V
 Cooler Voltage = 2.00 V
 Bias Voltage = 120.3 V
 Chopper Freq = 568.8 Hz

PUMP INFO
 Flow Rate = 4.624 L/M

DETECTOR INFO
 PUMP ON OFF
 MAX(V) 0.4144 0.4163
 MIN(V) 0.4128 0.4134

FILTER INFO
 Filter 1 0.415 Zero = true
 Filter 2 0.727 Zero = true
 Filter 3 1.524 Zero = true

CALIBRATION CHECK
 Xq = 0.1416 2.33%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration = 0.102 g/210L
 Lot # = 12-13-100
 Average = 0.096 g/210L
 Std Dev = 0.001

RFI Interference Test


RFI detected

Sample Acceptance Test

Passed

Reviewed on 2/1/12 BY SK, not in DMT log Passed Review Steven Harmon 2/1/12

within criteria passed 2-1-12

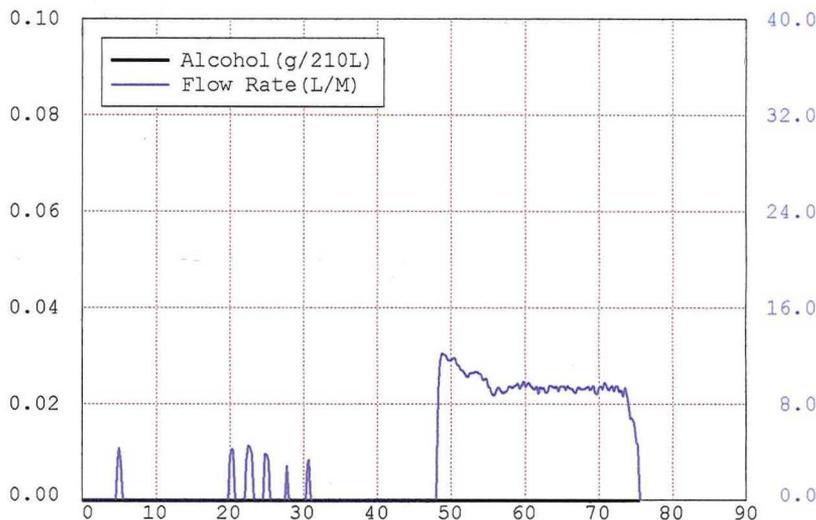

Instrument removed from site week of 1-9-12 and sent to NPAS

for on 1-18-12 KKK 2-1-12

Sub 2/1/12 4 pages attached
LT Dunn @ STAPd Reviewed? 2/1/12
(SK) 2/1/12

Performed by BO Mann

Date 11/18/2011

Reviewed by [Signature]

Date 11/18/2011

RECEIVED

NOV 02 2011

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 103206
Location: ST. ALBANS PD
Calibration Date: 03/18/2011
Certification Date: 03/18/2011
Installation Date: 03/18/2011
RPC Date: 10/28/2011
Supervisor Name: HOLLY B MOORE



Diagnostic Results

VERSIONS
DMT 1.05
PIC 2.06
Modem 1.06
Questions 1.00
Reports 1.02

TEMPERATURES
Sample Chamber = 48.68°C
Breath Tube = 47.53°C
Digital Sim = 33.8°C

SETTINGS
Lamp Voltage = 1.90 V
Cooler Voltage = 2.00 V
Bias Voltage = 120.3 V
Chopper Freq = 567.7 Hz

PUMP INFO
Flow Rate = 4.637 L/M

DETECTOR INFO
PUMP ON OFF
MAX(V) 0.4049 0.4061
MIN(V) 0.4010 0.4022

FILTER INFO
Filter 1 0.403 Zero = true
Filter 2 0.718 Zero = true
Filter 3 1.517 Zero = true

CALIBRATION CHECK
Xq = 0.1417 2.39%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration = 0.102 g/210L
Lot # = 12-13-100
Average = 0.098 g/210L
Std Dev = 0.000

RFI Interference Test


RFI detected

Sample Acceptance Test

Passed

Handwritten notes: SH 11-3-11, SH 11-3-11, SH 11-3-11, SH 11-3-11

Handwritten note: Check ->

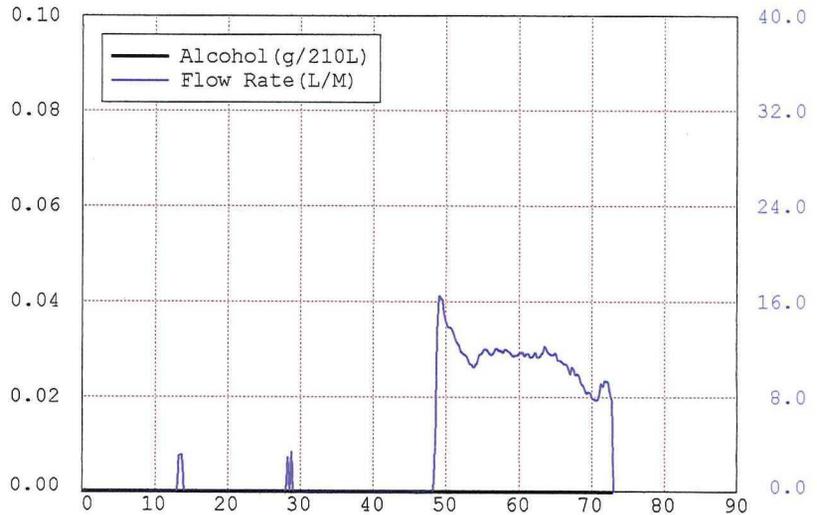

Handwritten note: email requesting Better representation of correct

Handwritten note: breathst 11-3-11

Handwritten note: DJB 2/1/12

Performed by: [Signature]

Date: 10/28/2011

Reviewed by: Steven Harrois

Date: 11-3-11

Harnois, Steven

From: Harnois, Steven
Sent: Thursday, November 03, 2011 7:30 AM
To: Holly Moore (hmoore@dps.state.vt.us)
Subject: Oct 2011 RPC
Officer Moore,

Thank You for completing your October 2011 RPC, The Breath Profile Provided does not satisfy the needs of the Health Department, please see the E-mail; sent May 23, 2011. To correct this please do a check-in on the datamaster and provide the four breaths as described in the May 23, 2011 E-mail.

If you need any assistance please call,

Thanks, Steve

Steven Harnois
State of Vermont
Agency Of Human Services
Department of Health
Public Health Electronics Technician
195 Colchester Avenue
Burlington, Vermont 05401
Phone (802) 863 7641
Fax (802) 863 7632

As part of the AHS Email Migration Project

My NEW E Mail: Steven.Harnois@state.vt.us



St. Albans Police Department

www.stalbanspd.com

30 Lower Welden Street, St. Albans, VT 05478

Telephone: (802) 524-2166

Fax: (802) 527-7778

FAX COVER SHEET

Date: November 18, 2011

To Vermont Department of Health
c/o Steven Harnois
195 Colchester, Vermont 05402-1125

Fax Number: (802) 863-7632

From: Saint Albans Police Department
30 Lower Welden Street
Saint Albans, Vermont 05478
(802) 524-2166 Phone
(802) 527-7778 Fax

Total number of pages, including the cover sheet - 2

If you do not receive all of the pages please call (802) 524-2167

Message: Stewie -

Original is to be sent out on Monday 11-21
after approval... Please refer to the email
I am sending you. - Thank you - Holly Malone
SAPD

Notice: The information contained in this facsimile transmittal is confidential information intended for the use of the individual or entity named above. If the reader of this message is not the intended recipient, or the employee of agent responsible to deliver it to the intended recipient, you are hereby notified that any dissemination, distribution or copying of this communication is strictly prohibited. If you have received this communication in error, please notify us immediately by telephone and return the original transmittal to us at the above address via the U.S. Postal service. Thank You.

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 103206
 Location: ST. ALBANS PD
 Calibration Date: 03/18/2011
 Certification Date: 03/18/2011
 Installation Date: 03/18/2011
 RPC Date: 11/18/2011
 Supervisor Name: HOLLY B MOORE



Diagnostic Results

VERSIONS

DMT 1.05
 PIC 2.06
 Modem 1.06
 Questions 1.00
 Reports 1.02

TEMPERATURES

Sample Chamber = 49.15°C
 Breath Tube = 47.64°C
 Digital Sim = 33.9°C

SETTINGS

Lamp Voltage = 1.90 V
 Cooler Voltage = 2.00 V
 Bias Voltage = 120.3 V
 Chopper Freq = 568.8 Hz

PUMP INFO

Flow Rate = 4.624 L/M

DETECTOR INFO

PUMP ON OFF
 MAX(V) 0.4144 0.4163
 MIN(V) 0.4128 0.4134

FILTER INFO

Filter 1 0.415 Zero = true
 Filter 2 0.727 Zero = true
 Filter 3 1.524 Zero = true

CALIBRATION CHECK

Xq = 0.1416 2.33%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.102 g/210L
 Lot # = 12-13-100
 Average = 0.096 g/210L
 Std Dev = 0.001

RFI Interference Test

RFI detected

Sample Acceptance Test

Passed

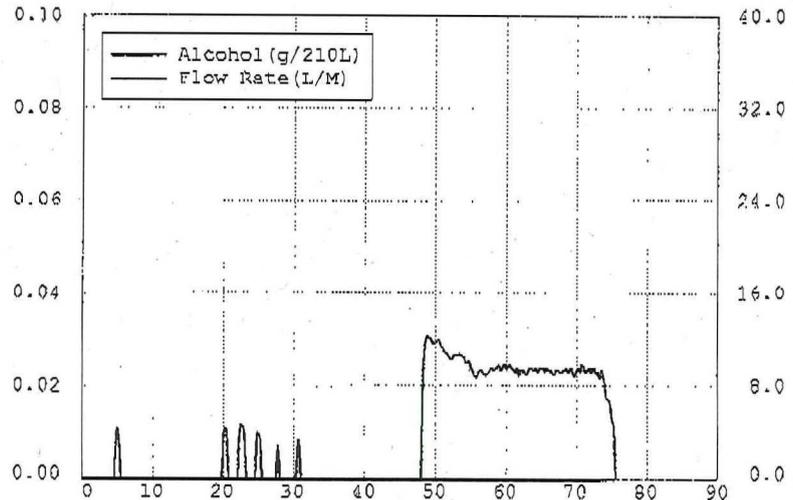

Performed by BOY

Date 11/18/2011

Reviewed by _____

Date _____