Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
10/06/2012	21:44:56	SWANTON PD	MICHAEL S AHER	REFUSED		0.096		
11/04/2012	18:35:15	SWANTON PD	DEAN M SCOTT	INTERFERENCE		0.100		
11/04/2012	19:02:55	SWANTON PD	DEAN M SCOTT	INTERFERENCE		0.099		
11/04/2012	19:28:23	SWANTON PD	DEAN M SCOTT	INTERFERENCE		0.100		RESPONSE TIMEOUT
11/04/2012	21:08:29	SWANTON PD	D G	0.000		0.100		

Log On Record History

Test Date	Test Time	Name

Status Record History

Status Date	Status Time	Test Type	Status Message
07/10/2012	19:56:20	DUI Subject Record	RESPONSE TIMEOUT
07/10/2012	20:05:59	DUI Subject Record	RESPONSE TIMEOUT
08/05/2012	00:47:55	DUI Subject Record	RESPONSE TIMEOUT
11/04/2012	19:32:36	DUI Subject Record	RESPONSE TIMEOUT

ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMater DMT: 121506
Location: Swanton PD

Date: 11/04/2012
Time: 21:28:51

SUPERVISOR NAME:
DONALD M GILBERT

SOLUTION LOT #: 12-51-100
SOLUTION CONCENTRATION: 0.100

BLANK TEST	0.000	21:29
CALIBRATION CHECK	PASSED	21:29
SIMULATOR VAPOR 34.0°C	0.099	21:30
SIMULATOR VAPOR 34.0°C	0.100	21:31
SIMULATOR VAPOR 34.0°C	0.100	21:32
SIMULATOR VAPOR 34.0°C	0.101	21:33
SIMULATOR VAPOR 34.0°C	0.100	21:34
SIMULATOR VAPOR 34.0°C	0.101	21:35
SIMULATOR VAPOR 33.9°C	0.100	21:36
SIMULATOR VAPOR 34.0°C	0.101	21:37
SIMULATOR VAPOR 34.0°C	0.101	21:38
SIMULATOR VAPOR 34.0°C	0.100	21:39
BLANK TEST	0.000	21:40

Average = 0.100
Std Dev = 0.000

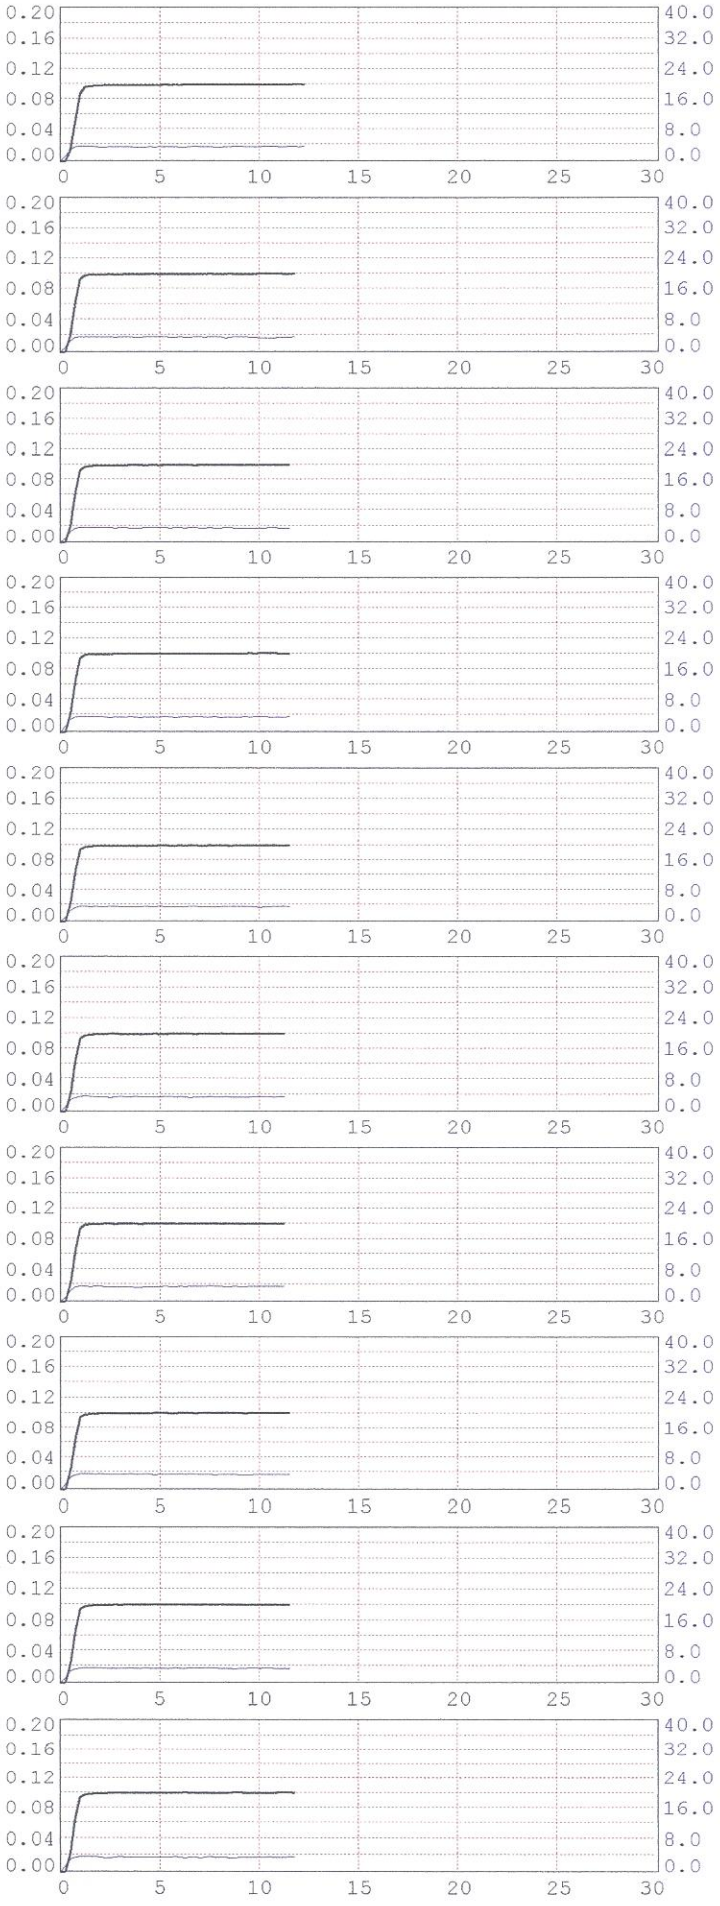

DIAGNOSTIC RESULT

DataMaster DMT: 121506
Location: Swanton PD
Calibration Date: 01/06/2012
Certification Date: 01/06/2012
Installation Date: 01/27/2012
Test Date: 11/04/2012
Test Time: 21:48:45

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 42.0°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.79 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 545 Hz

PUMP INFO
Flow Rate = 4.700 L/M

DETECTOR INFO
PUMP     ON         OFF
MAX(V)    0.2886     0.2904
MIN(V)    0.2870     0.2884

FILTER INFO
Filter 1   0.290  Zero = true
Filter 2   1.031  Zero = true
Filter 3   0.992  Zero = true

CALIBRATION CHECK
Xq  = 0.096  0.55%
```

DIAGNOSTIC RESULT

DataMaster DMT: 121506
Location: Swanton PD
Calibration Date: 01/06/2012
Certification Date: 01/06/2012
Installation Date: 01/27/2012
Test Date: 11/04/2012
Test Time: 21:24:36

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 46.3°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.79 V
Cooler Voltage = 1.77 V
Bias Voltage = 81 V
Chopper Freq = 547 Hz

PUMP INFO
Flow Rate = 4.671 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.2724	0.2748
MIN(V)	0.2707	0.2730

FILTER INFO
Filter 1 0.273 Zero = true
Filter 2 1.014 Zero = true
Filter 3 0.970 Zero = true

CALIBRATION CHECK
Xq = 0.095 1.09%