ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 121506
Location: Swanton PD
Calibration Date: 01/06/2012
Certification Date: 01/06/2012
Installation Date: 01/27/2012
APM Date: 01/11/2013
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.2°C
Breath Tube    = 47.3°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.79 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 548 Hz

PUMP INFO
Flow Rate = 4.822 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3242    0.3266
MIN(V)   0.3220    0.3250

FILTER INFO
Filter 1   0.325   Zero = true
Filter 2   1.054   Zero = true
Filter 3   1.008   Zero = true

CALIBRATION CHECK
Xq  = 0.095  1.36%
```

Simulator Vapor Test

Concentration = 0.100 g/210L
Lot # = 12-51-100
Range = 0.095 - 0.105
Simulator Vapor = 0.097 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

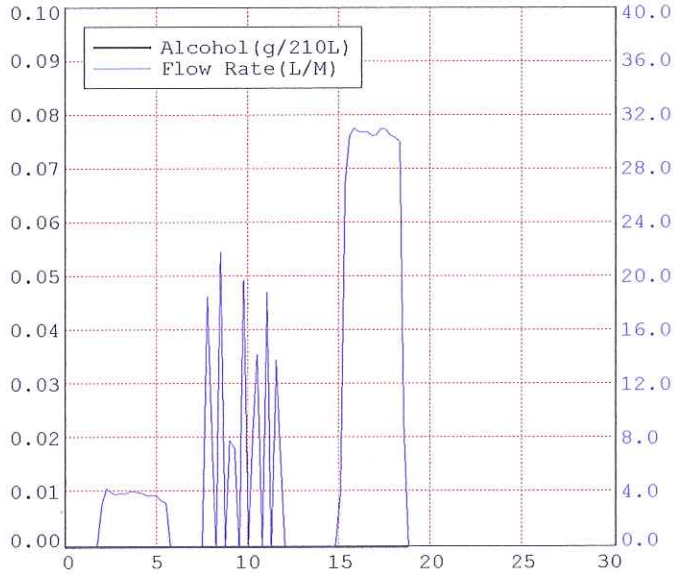

APM PASSED

NIST thermometer S/N 111814522 34.0°C
RCD 1/11/13

Performed by _____ Date 01/11/2013

Reviewed by _____ Date 1/15/2013