ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100135
Location: Franklin County SO St Albans
Calibration Date: 01/26/2012
Certification Date: 01/27/2012
Installation Date: 02/03/2012
RPC Date: 06/17/2013
Supervisor Name: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 44.7°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.83 V
Cooler Voltage = 1.79 V
Bias Voltage   = 80 V
Chopper Freq   = 533 Hz

PUMP INFO
Flow Rate = 5.967 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2563    0.2606
MIN(V)   0.2549    0.2589

FILTER INFO
Filter 1   0.260  Zero = true
Filter 2   0.536  Zero = true
Filter 3   0.810  Zero = true

CALIBRATION CHECK
Xq  = 0.087  0.20%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-04-100
Range	= 0.094 - 0.104
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

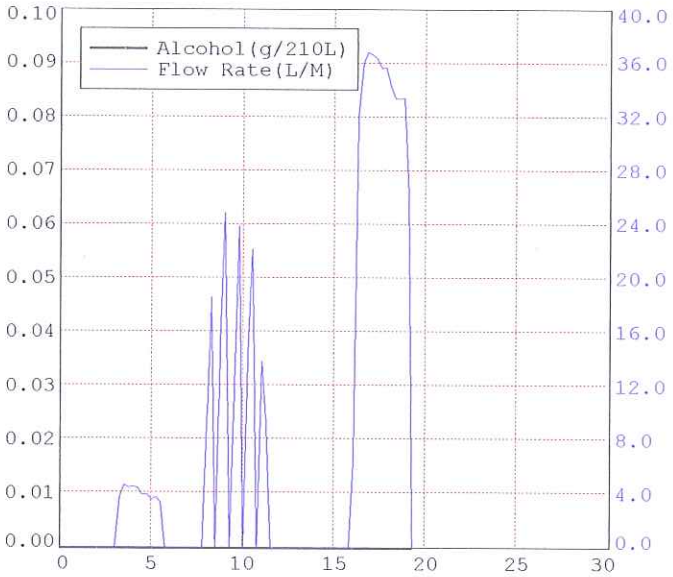

Performed by RCD Date 06/17/2013

Reviewed by Date 6/27/2013