ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 100137
Location: Grand Isle County SO
Calibration Date: 01/26/2012
Certification Date: 01/27/2012
Installation Date: 02/03/2012
APM Date: 01/10/2014
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.3°C
Breath Tube    = 47.3°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.59 V
Cooler Voltage = 1.61 V
Bias Voltage   = 80 V
Chopper Freq   = 539 Hz

PUMP INFO
Flow Rate = 5.664 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2890    0.2929
MIN(V)   0.2878    0.2917

FILTER INFO
Filter 1   0.293  Zero = true
Filter 2   0.552  Zero = true
Filter 3   0.726  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.95%
```

Simulator Vapor Test

Concentration = 0.100 g/210L
Lot # = 13-13-100
Range = 0.095 - 0.105
Simulator Vapor = 0.096 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

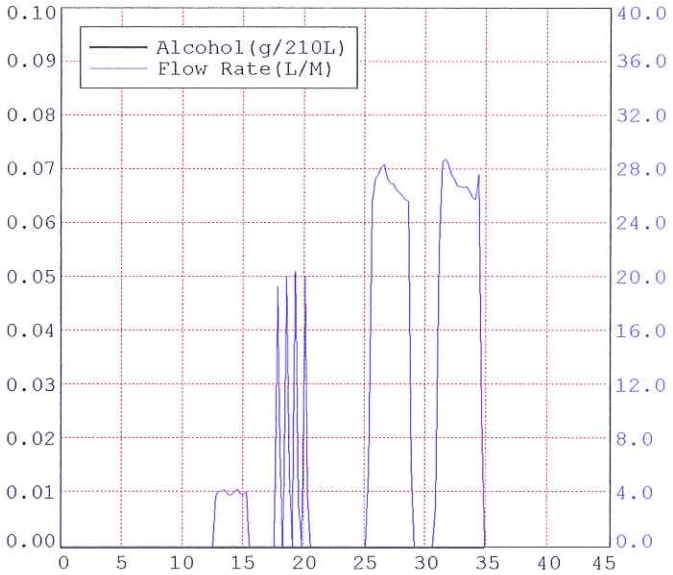

APM PASSED

NIST Thermometer s/n 111814517 34.1°C RCD 1/10/14

Performed by RCD Date 01/10/2014

Reviewed by Date 1/14/14