ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100137
Location: Grand Isle County SO
Calibration Date: 01/26/2012
Certification Date: 01/27/2012
Installation Date: 02/03/2012
RPC Date: 06/03/2014
Supervisor Name: BLAKE R ALLEN

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.59 V
Cooler Voltage = 1.61 V
Bias Voltage = 80 V
Chopper Freq = 539 Hz

PUMP INFO
Flow Rate = 5.545 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.3844	0.3866
MIN(V)	0.3835	0.3856

FILTER INFO
Filter 1 0.386 Zero = true
Filter 2 0.648 Zero = true
Filter 3 0.830 Zero = true

CALIBRATION CHECK
Xq = 0.084 2.12%

Accuracy and Precision Check

Concentration = 0.099 g/210L
Lot # = 14-01-100
Range = 0.094 - 0.104
Average = 0.097 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

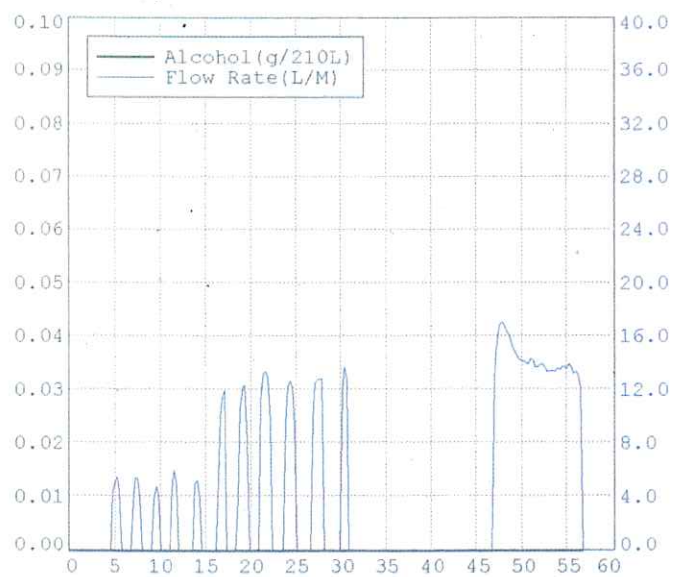

Routine Performance Check Passed

Performed by _____ Date 06/03/2014

Reviewed by _____ Date 6/11/14

6/11/2014