ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100134
Location: Morristown PD
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 02/09/2012
RPC Date: 06/02/2013
Supervisor Name: SCOTT N MCCULLOUGH

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 42.5°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.66 V
Cooler Voltage = 1.66 V
Bias Voltage   = 80 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 5.632 L/M

DETECTOR INFO
PUMP     ON       OFF
MAX(V)   0.2427   0.2467
MIN(V)   0.2413   0.2453

FILTER INFO
Filter 1   0.246   Zero = true
Filter 2   0.755   Zero = true
Filter 3   0.895   Zero = true

CALIBRATION CHECK
Xq  = 0.084  0.10%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

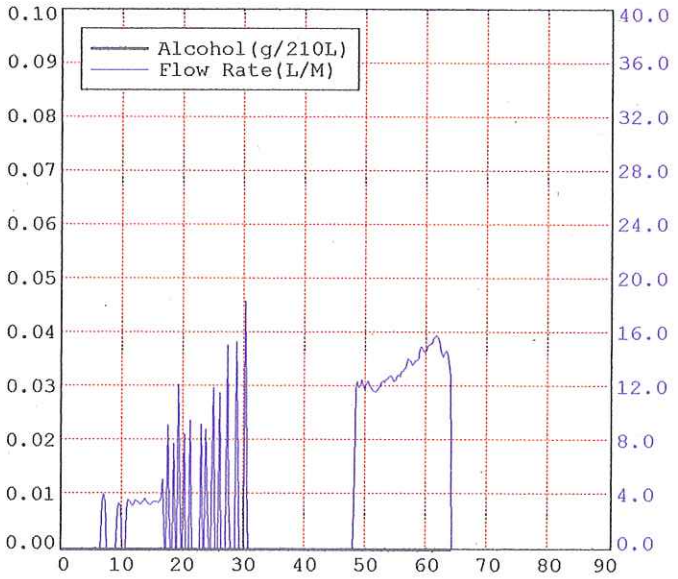

Performed by _____ Date 06/02/2013

Reviewed by _____ Date 8/7/13

8/7/2013

Page 1 of 3 KCD

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100134
Location: Morristown PD
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 02/09/2012
RPC Date: 06/02/2013
Supervisor Name: SCOTT N MCCULLOUGH

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 42.5°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.66 V
Cooler Voltage = 1.66 V
Bias Voltage = 80 V
Chopper Freq = 534 Hz

PUMP INFO
Flow Rate = 5.632 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.2427	0.2467
MIN(V)	0.2413	0.2453

FILTER INFO

Filter 1	0.246	Zero = true
Filter 2	0.755	Zero = true
Filter 3	0.895	Zero = true

CALIBRATION CHECK
Xq = 0.084 0.10%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

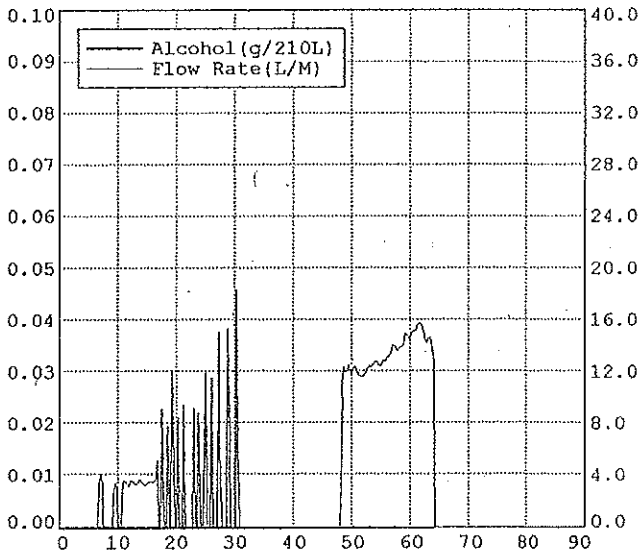

* Color copy has been sent via mail

Performed by _____ Date 06/02/2013

Reviewed by _____ Date 7/8/13

2 of 3 RCO

Driscoll, Rob

From: Reeve, Michael
Sent: Monday, July 08, 2013 3:55 PM
To: Driscoll, Rob

Rob,

Scott McCullough did the one for the Morristown PD site the first week in June. I thought he mailed you the report. I will reprint and resend via fax and mail to you.

Michael Reeve
Corporal
Morristown Police Department
Phone: 802-888-4211
Fax: 802-888-4044