INSTALLATION REPORT

DataMaster DMT: 103406
Location: Orleans County SO
Calibration Date: 02/22/2012
Certification Date: 02/22/2012
Installation Date: 07/17/2014
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.74 V
Cooler Voltage = 2.04 V
Bias Voltage   = 120 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 3.933 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1268    0.1287
MIN(V)   0.1250    0.1272

FILTER INFO
Filter 1   0.127  Zero = true
Filter 2   0.934  Zero = true
Filter 3   0.257  Zero = true

CALIBRATION CHECK
Xq  = 0.123  0.65%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-04-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

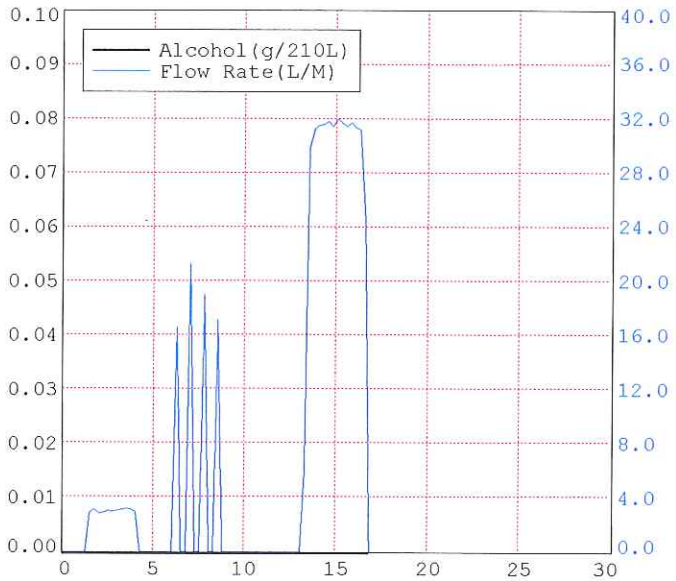

INSTALLATION PASSED

NIST Thermometer S/N 111814517 34.0°C RCD 7/17/14

Performed by RCD Date 07/17/2014

Reviewed by Date 7/17/2014