INSTALLATION REPORT

DataMaster DMT:	100147
Location:	VFL
Calibration Date:	08/06/2013
Certification Date:	08/06/2013
Installation Date:	08/14/2013
Installed by:	ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 46.6°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.53 V
Cooler Voltage = 1.53 V
Bias Voltage   = 80 V
Chopper Freq   = 535 Hz

PUMP INFO
Flow Rate = 5.957 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0352   -0.0299
MIN(V)   -0.0362   -0.0311

FILTER INFO
Filter 1  -0.030  Zero = true
Filter 2   0.457  Zero = true
Filter 3   1.250  Zero = true

CALIBRATION CHECK
Xq  = 0.117  0.61%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 13-13-100
Range	= 0.095 - 0.105
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

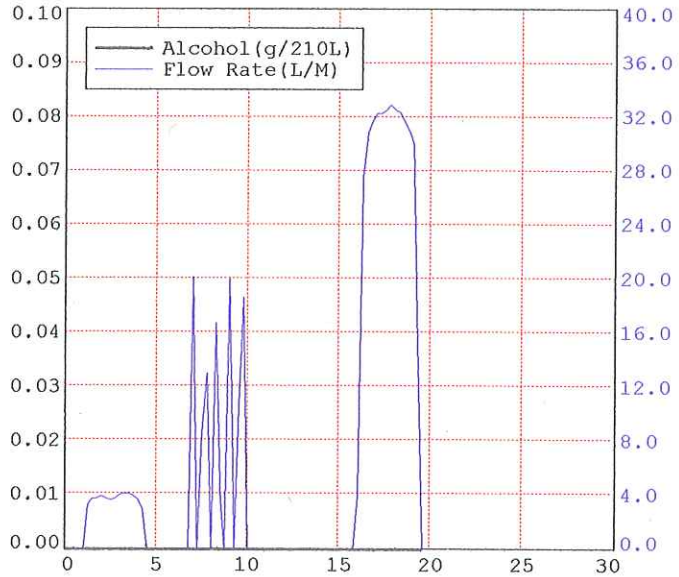

INSTALLATION PASSED

Performed by RCD Date 08/14/2013

Reviewed by Date 8/15/2013