INSTALLATION REPORT

DataMaster DMT: 121706
Location: VPA
Calibration Date: 07/27/2012
Certification Date: 07/27/2012
Installation Date: 12/02/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.5°C
Breath Tube    = 43.3°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.77 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 538 Hz

PUMP INFO
Flow Rate = 5.877 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.1004   -0.0957
MIN(V)   -0.1022   -0.0974

FILTER INFO
Filter 1  -0.097  Zero = true
Filter 2   0.549  Zero = true
Filter 3   0.184  Zero = true

CALIBRATION CHECK
Xq  = 0.092  2.14%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-19-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

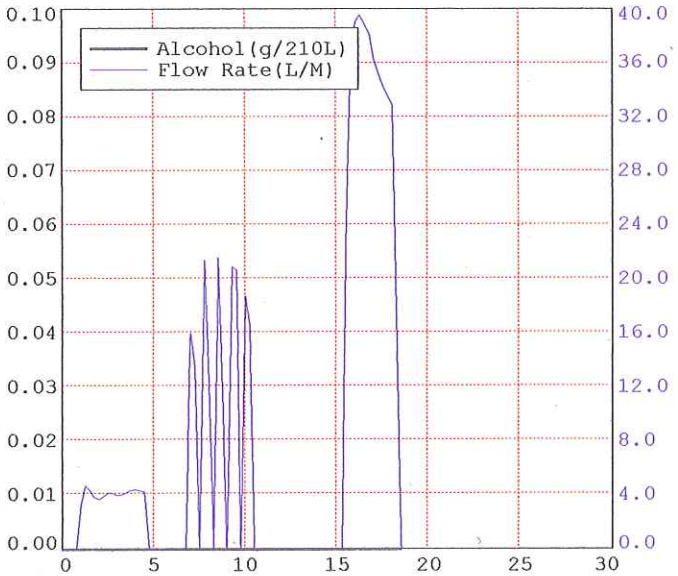

INSTALLATION PASSED

Performed by ROD **Date** 12/02/2013

Reviewed by **Date** 12/3/2013