ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100148
Location: Berlin PD
Calibration Date: 11/09/2011
Certification Date: 11/14/2011
Installation Date: 12/08/2011
RPC Date: 06/11/2014
Supervisor Name: MARK A MONTEITH

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.64 V
Cooler Voltage = 1.69 V
Bias Voltage   = 80 V
Chopper Freq   = 542 Hz

PUMP INFO
Flow Rate = 5.853 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3321    0.3344
MIN(V)   0.3305    0.3325

FILTER INFO
Filter 1   0.333  Zero = true
Filter 2   0.672  Zero = true
Filter 3   0.545  Zero = true

CALIBRATION CHECK
Xq  = 0.085  1.36%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-01-100
Range	= 0.094 - 0.104
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

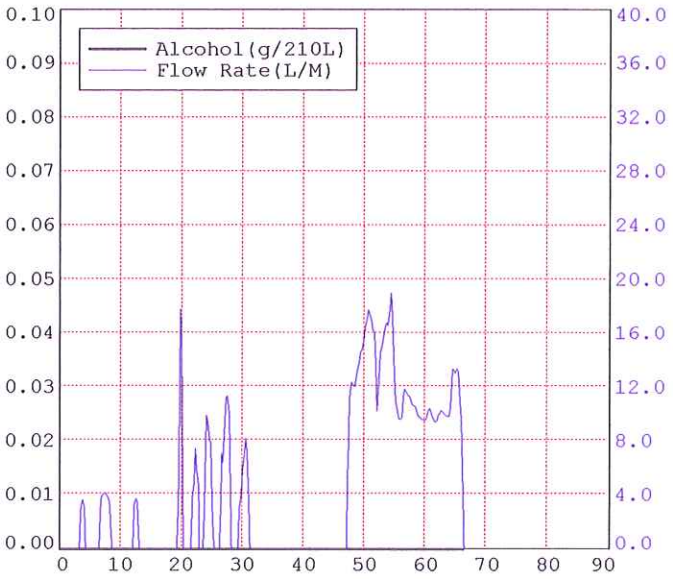

Performed by Mark Monteith **Date** 06/11/2014

Reviewed by _____ **Date** 6/17/14 6/17/2014