

ROUTINE PERFORMANCE CHECK REPORT



RECEIVED

NOV 06 2012

WCSA

DataMaster DMT: 100141
Location: Vernon PD
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 02/08/2012
RPC Date: 11/05/2012
Supervisor Name: BRUCE D GAULD

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 48.1°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage = 81 V
Chopper Freq = 538 Hz

PUMP INFO

Flow Rate = 6.058 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0057	0.0075
MIN (V)	0.0041	0.0059

FILTER INFO

Filter 1	0.006	Zero = true
Filter 2	0.316	Zero = true
Filter 3	0.620	Zero = true

CALIBRATION CHECK

Xq = 0.082 0.64%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 12-80-100
Range = 0.094 - 0.104
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

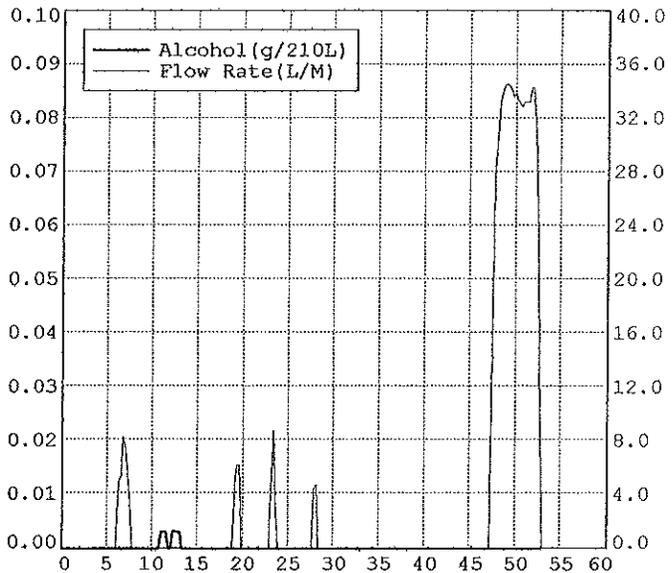

Performed by Bruce D Gauld

Date 11/05/2012

Reviewed by _____

Date _____



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 100141
Location: Vernon PD
Certification Date: 01/31/2012
Installation Date: 02/08/2012


Date: 11/05/2012
Time: 14:41:14

SUBJECT NAME:
BRUCE D GAULD
DOB: 06/25/1952 AGE: 60
GENDER: M

TEST OPERATOR NAME:
BRUCE D GAULD
AGENCY: VERNON PD

BLANK TEST	0.000	14:42
CALIBRATION CHECK	PASSED	14:42
SIMULATOR VAPOR 34.1°C	0.100	14:42
SUBJECT SAMPLE (Vol=2.4L)	0.000	14:43
BLANK TEST	0.000	14:44

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.099
Sim. Vapor Range 0.094 - 0.104
Lot #: 12-80-100

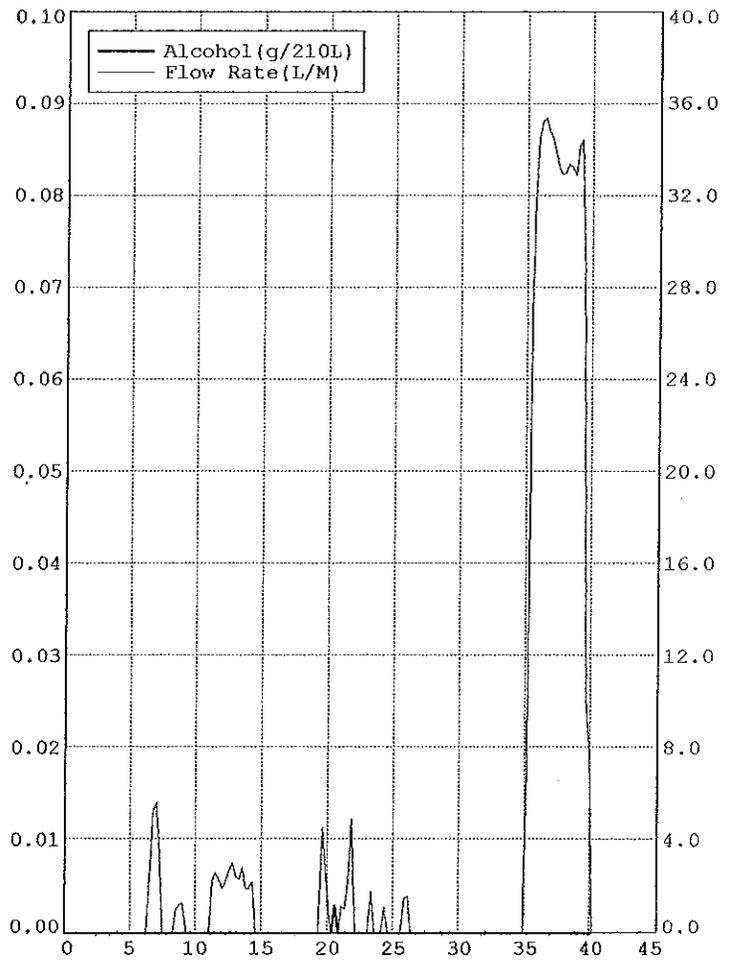



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 100141
Location: Vernon PD
Certification Date: 01/31/2012
Installation Date: 02/08/2012


Date: 11/05/2012
Time: 14:48:35

SUBJECT NAME:
BRUCE D GAULD
DOB: 06/25/1952 AGE: 60
GENDER: M

TEST OPERATOR NAME:
BRUCE D GAULD
AGENCY: VERNON PD

BLANK TEST	0.000	14:49
CALIBRATION CHECK	PASSED	14:49
SIMULATOR VAPOR 34.1°C	0.100	14:49
SUBJECT SAMPLE (Vol=2.3L)	0.000	14:51
BLANK TEST	0.000	14:51

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.099
Sim. Vapor Range 0.094 - 0.104
Lot #: 12-80-100

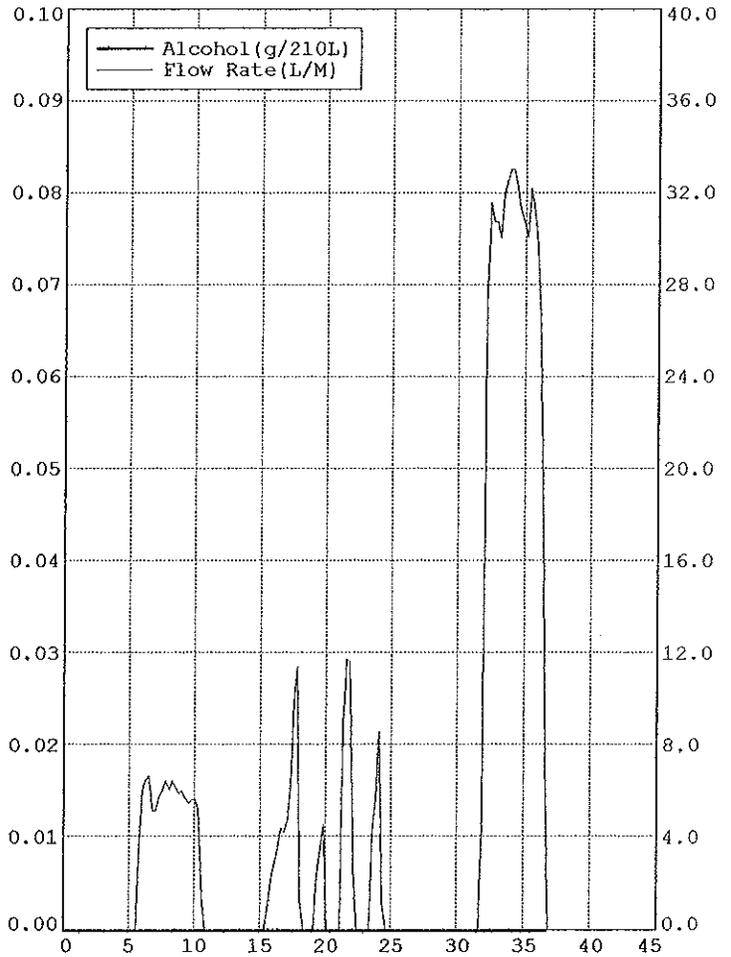



Vernon Police Department

P.O. Box 63 567 Governor Hunt RD
Vernon, VT 05354
Office: 802-257-2638 Fax: 802-258-2328



RECEIVED
JUN 27 2012
WCSEA

TO: SA's office	FROM: Sgt. Cowley
ATTN: Steve Brown	PAGES: 3
FAX:	FAX: 802-258-2328
PHONE:	PHONE: 802-257-2638
CC:	
RE:	

Steve
Here are the other reports you were looking for. They are blank.

Status Record History

Status Date	Status Time	Test Type	Status Message
06/27/2012	13146:17	RPC Record	RF NOT DETECTED

Brown, Steven

From: Hebert, MaryBeth
Sent: Monday, June 25, 2012 10:31 AM
To: Brown, Steven
Subject: RE: DataMaster Records

Hi Steve. I will forward your request along to Sgt. Gauld.

Thank you.

MB

Chief MB Hebert
Vernon Police Dept.
567 Governor Hunt Road
Vernon, VT 05354
802-257-2638

From: Brown, Steven
Sent: Monday, June 25, 2012 9:12 AM
To: Hebert, MaryBeth
Subject: FW: DataMaster Records

MaryBeth,

Today I received the RPC and the a copy of your log book. Thank you.

However, as I have been requesting, I do not have copies of the following documents since your DM was installed:

Breath Summary Report
Status Summary Report

Thanks,

Steve

Steven M Brown
Windham County Deputy State's Attorney
P O. Box 785
Brattleboro, VT 05302
802 257 2860 voice
802 257 2864 fax

From: Brown, Steven
Sent: Friday, June 08, 2012 8:45 AM
To: Szarejko, Joseph M.; Hopkins, Richmond; Edwards, Robert; Favreau, Paul; Lake, Ronald; Hebert, MaryBeth; 'Keith Clark'; Wrinn, Eugene
Cc: Shriver, Tracy; Cay, Susan; Gartenstein, David
Subject: DataMaster Records

Hello,

Would you please remind your DM Supervisors they need to send updated records to our office. This is not optional. At a minimum, we should be receiving quarterly updates which should include:

Breath Summary Report
Status Summary Report
Check Up and Maintenance Log
RPCs
Simulator Change Reports
Any other related records, including emails

List below is the last time I received an update from each agency:

Windham County Sheriffs **11/28/11**
Dover PD **2/17/11**
VSP Rockingham **2/17/12**
VSP Brattleboro **12/15/11**
Bellow Falls PD **11/14/11**
Vernon PD **2/15/12**
Wilmington PD **No updates since the instrument has been replaced**
Brattleboro PD- **up to date**

Please let me know if you have any questions.

SMB

Steven M. Brown
Windham County Deputy State's Attorney
P O Box 785
Brattleboro, VT 05302
802 257 2860 voice
802 257 2864 fax

Brown, Steven

From: Brown, Steven
Sent: Monday, June 25, 2012 9:13 AM
To: Hebert, MaryBeth
Subject: FW: DataMaster Records

MaryBeth,

Today I received the RPC and the a copy of your log book. Thank you.

However, as I have been requesting, I do not have copies of the following documents since your DM was installed:

Breath Summary Report
Status Summary Report

Thanks,

Steve

Steven M. Brown
Windham County Deputy State's Attorney
P. O. Box 785
Brattleboro, VT 05302
802 257 2860 voice
802 257 2864 fax

From: Brown, Steven
Sent: Friday, June 08, 2012 8:45 AM
To: Szarejko, Joseph M.; Hopkins, Richmond; Edwards, Robert; Favreau, Paul; Lake, Ronald; Hebert, MaryBeth; 'Keith Clark'; Wrinn, Eugene
Cc: Shriver, Tracy; Cay, Susan; Gartenstein, David
Subject: DataMaster Records

Hello,

Would you please remind your DM Supervisors they need to send updated records to our office. This is not optional. At a minimum, we should be receiving quarterly updates which should include:

Breath Summary Report
Status Summary Report
Check Up and Maintenance Log
RPCs
Simulator Change Reports
Any other related records, including emails

List below is the last time I received an update from each agency:

Windham County Sheriffs **11/28/11**
Dover PD **2/17/11**
VSP Rockingham **2/17/12**
VSP Brattleboro **12/15/11**
Bellow Falls PD **11/14/11**
Vernon PD **2/15/12**
Wilmington PD **No updates since the instrument has been replaced**
Brattleboro PD- **up to date**

Please let me know if you have any questions.

SMB

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100141
Location: Vernon PD
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 02/08/2012
RPC Date: 06/23/2012
Supervisor Name: BRUCE GAULD

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 46.4°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage = 81 V
Chopper Freq = 537 Hz

PUMP INFO

Flow Rate = 5.938 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.0173	-0.0148
MIN (V)	-0.0187	-0.0163

FILTER INFO

Filter 1	-0.016	Zero = true
Filter 2	0.297	Zero = true
Filter 3	0.594	Zero = true

CALIBRATION CHECK

Xq = 0.081 0.74%


Routine Performance Check Passed

A
Con
Lot
Rang
Avera
Std Dev

RF Det
Passed

Sample Ac
Passed

RECEIVED
JUN 25 2012
WCSA

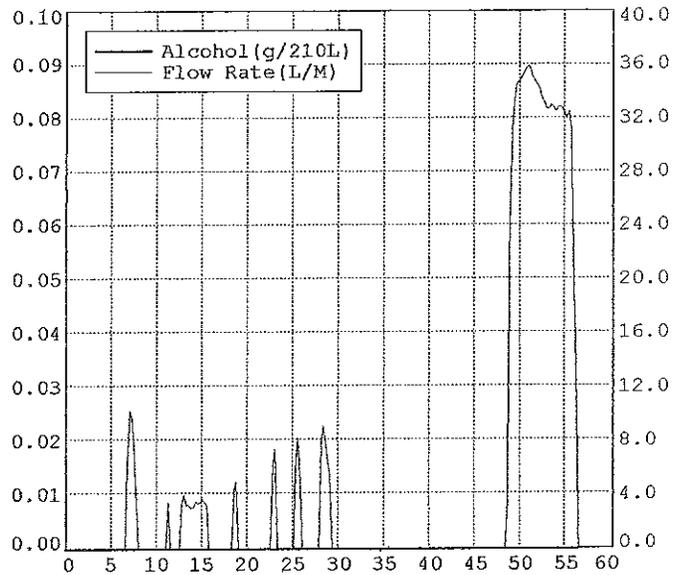

Performed by

Bruce Gauld

Date

06/23/2012

Reviewed by

Date

DATAMASTER DMT MAINTENANCE LOG

Vernon PD

Department/Agency

100/41

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2-8-12	<p>DataMaster Simulator Solution Lot # 12-51-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 01/12/2012 Expires: 01/12/2013</p> <p>[For RI Place Label Here]</p> <p>OPENED: 2-8-12 <i>WAK</i></p> <p style="text-align: center; font-size: 1.2em;">Install Per Protocol</p>	<p style="font-size: 1.5em;">Steven</p> <p>Harnois Kirk Kinball VDHK Chief</p>
4/10/12	<p>Replaced Simulator due to [For RPC or Simulator Solution Change Place Label Here] temperature issues. Performed A+P test on solution already in jar (see above) Temp checked by ALB + SMB</p>	<p style="font-size: 1.5em;">A. Bolo</p>
6/23/12	<p>[For RPC Simulator Solution Change Place Label Here]</p> <p>DataMaster Simulator Solution Lot # 12-51-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 01/12/2012 Expires: 01/12/2013</p> <p>OPENED: 6/23/12</p>	<p style="font-size: 1.5em;">Bunce</p>
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	

Brown, Steven

From: Brown, Steven
Sent: Friday, June 08, 2012 8:45 AM
To: Szarejko, Joseph M.; Hopkins, Richmond; Edwards, Robert; Favreau, Paul; Lake, Ronald; Hebert, MaryBeth; 'Keith Clark'; Wrinn, Eugene
Cc: Shriver, Tracy; Cay, Susan; Gartenstein, David
Subject: DataMaster Records

Hello,

Would you please remind your DM Supervisors they need to send updated records to our office. This is not optional. At a minimum, we should be receiving quarterly updates which should include:

Breath Summary Report
Status Summary Report
Check Up and Maintenance Log
RPCs
Simulator Change Reports
Any other related records, including emails

List below is the last time I received an update from each agency:

Windham County Sheriffs **11/28/11**
Dover PD **2/17/11**
VSP Rockingham **2/17/12**
VSP Brattleboro **12/15/11**
Bellow Falls PD **11/14/11**
Vernon PD **2/15/12**
Wilmington PD **No updates since the instrument has been replaced**
Brattleboro PD- **up to date**

Please let me know if you have any questions.

SMB

Steven M. Brown
Windham County Deputy State's Attorney
P.O. Box 785
Brattleboro, VT 05302
802.257.2860 voice
802.257.2854 fax



VERNON POLICE DEPARTMENT

P.O. Box 63 Governor Hunt Road Vernon, Vermont 05354

Office: 802-257-2638 Dispatch: 802-254-6962 Fax: 802-258-2328

Fax Cover Sheet

To: Steve Brown

Date: 2/15/12

From: Bruce Gauld

No. of pages: 3 (including cover sheet)

Re: Data Master

Fax #: _____

Comments: Steve we just got our Data Master back.

If transmission is received incomplete or illegible please contact the undersigned immediately at 802-257-2638. Thank you.

Fax operator: Bruce Gauld

Community Policing

D.A.R.E.

Neighborhood Watch

DATAMASTER DMT MAINTENANCE LOG

Vernon PD

Department/Agency

100/41

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2-8-12	<p><u>DataMaster Simulator Solution</u> Lot # 12-51-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 [face Label Here] Preparation Date: 01/12/2012 Expires: 01/12/2013 OPBNEED: 2-8-12 <i>KK</i> Install Per Protocol 11</p>	<p>Steven Harnois KKK Kimball VDHK Chief</p>
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	

