INSTALLATION REPORT

DataMaster DMT: 100161
Location: Brattleboro VSP
Calibration Date: 02/04/2013
Certification Date: 02/04/2013
Installation Date: 02/05/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.2°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.77 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 529 Hz

PUMP INFO
Flow Rate = 5.535 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0181    0.0213
MIN(V)   0.0161    0.0197

FILTER INFO
Filter 1   0.021  Zero = true
Filter 2   0.340  Zero = true
Filter 3   0.497  Zero = true

CALIBRATION CHECK
Xq  = 0.086  1.12%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-80-100
Range	= 0.094 - 0.104
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

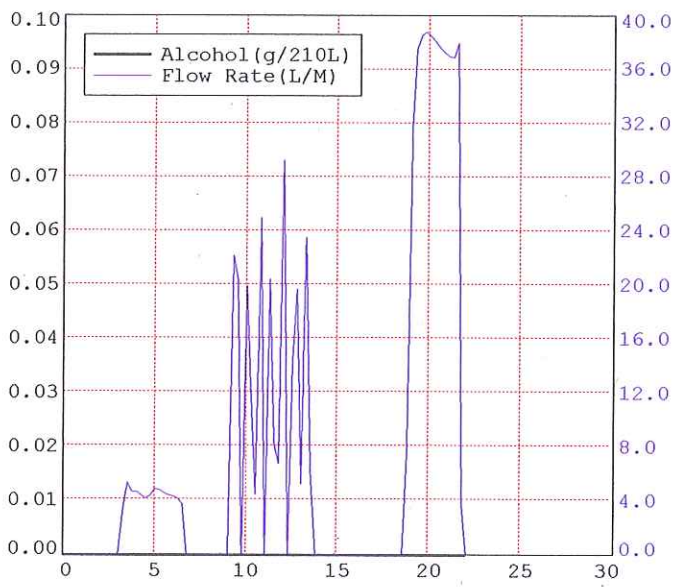

INSTALLATION PASSED

Performed by RCD **Date** 02/05/2013

Reviewed by **Date** 2/11/2013

Status Record History

Status Date	Status Time	Test Type	Status Message
02/05/2013	11:46:33	Installation Record	User Abort
			Aborted by mistake during 30 min. wait period. RCD 2/5/13
			2 of 2 RCD