ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 123006
Location: Rockingham VSP
Calibration Date: 05/18/2012
Certification Date: 05/18/2012
Installation Date: 05/21/2012
APM Date: 08/22/2014
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 47.8°C
Digital Sim    = 34.2°C

SETTINGS
Lamp Voltage   = 1.76 V
Cooler Voltage = 1.69 V
Bias Voltage   = 80 V
Chopper Freq   = 538 Hz

PUMP INFO
Flow Rate = 4.824 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3148    0.3185
MIN(V)   0.3136    0.3171

FILTER INFO
Filter 1   0.318  Zero = true
Filter 2   0.754  Zero = true
Filter 3   1.444  Zero = true

CALIBRATION CHECK
Xq  = 0.118  0.30%
```

Simulator Vapor Test

Concentration	= 0.099 g/210L
Lot #	= 13-21-100
Range	= 0.094 - 0.104
Simulator Vapor	= 0.099 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

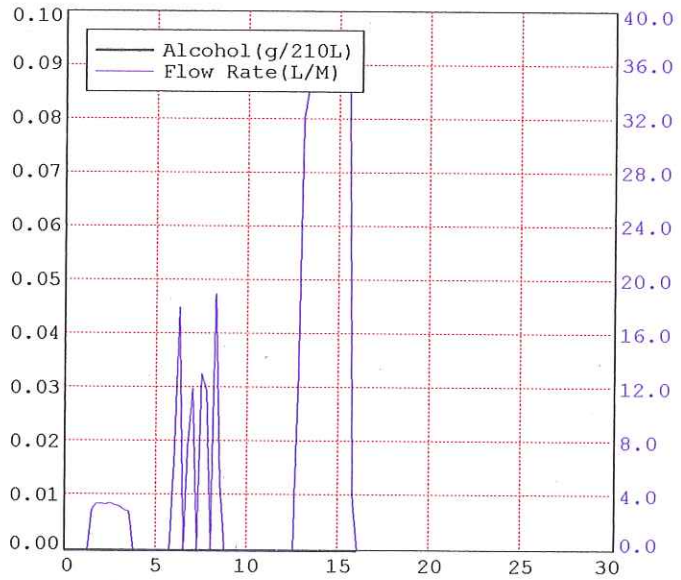

APM PASSED

NIST Thermometer S/N 111814517 34.2°C
Also, Replaced Broken Stylus RCD 8/22/14

Performed by RCD **Date** 08/22/2014

Reviewed by TLGA **Date** 8/25/2014