ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100160
Location: Rochester
Calibration Date: 10/18/2011
Certification Date: 10/19/2011
Installation Date: 10/28/2011
RPC Date: 10/21/2012
Supervisor Name: TOM SIMPSON

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.80 V
Cooler Voltage = 1.66 V
Bias Voltage   = 80 V
Chopper Freq   = 540 Hz

PUMP INFO
Flow Rate = 6.330 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.2116   -0.2073
MIN(V)   -0.2150   -0.2116

FILTER INFO
Filter 1  -0.208  Zero = true
Filter 2   0.001  Zero = true
Filter 3   1.364  Zero = true

CALIBRATION CHECK
Xq  = 0.087  0.00%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-58-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

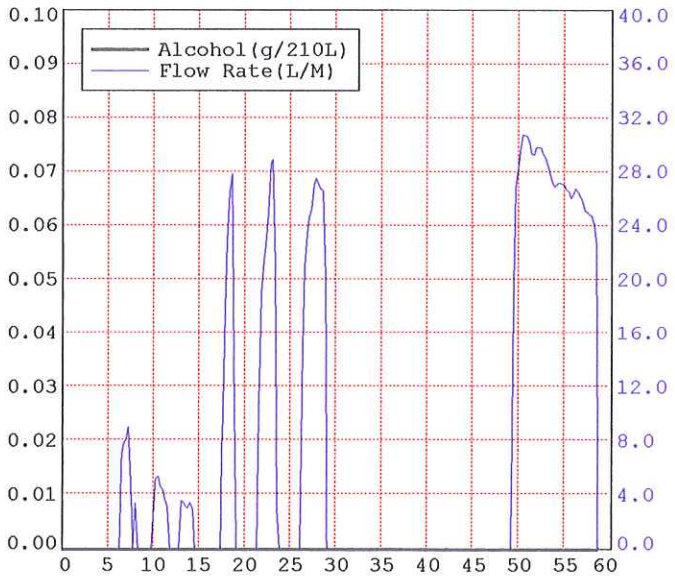

Performed by Tom Simpson Date 10/21/2012

Reviewed by Date 10/24/12

10/24/2012