ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 104309
Location: Windsor PD
Calibration Date: 09/08/2011
Certification Date: 09/08/2011
Installation Date: 09/20/2011
RPC Date: 10/30/2013
Supervisor Name: JONATHAN J ADAMS

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 43.5°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.67 V
Cooler Voltage = 1.79 V
Bias Voltage   = 80 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 6.019 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1870    0.1898
MIN(V)   0.1858    0.1882

FILTER INFO
Filter 1   0.190   Zero = true
Filter 2   0.463   Zero = true
Filter 3   0.221   Zero = true

CALIBRATION CHECK
Xq  = 0.085  0.93%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-04-100
Range	= 0.094 - 0.104
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

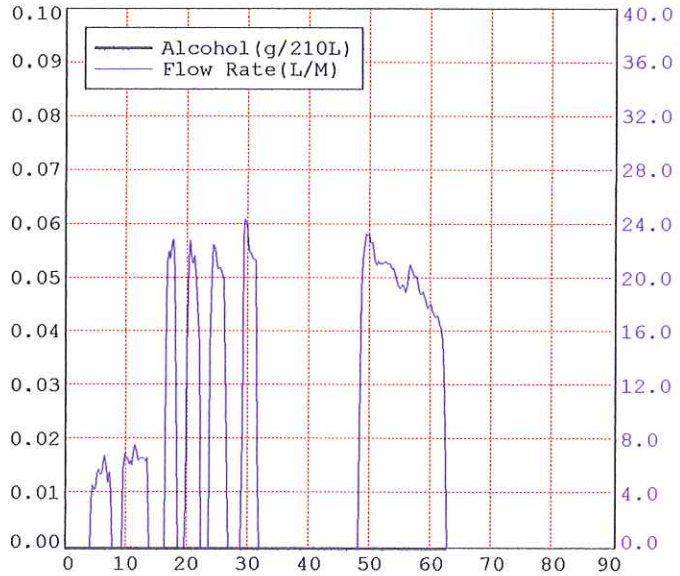

Performed by _____ **Date** 10/30/2013

Reviewed by _____ **Date** 11/1/13

11/4/2013