INSTALLATION REPORT

DataMaster DMT: 104509
Location: Ludlow PD
Calibration Date: 11/06/2013
Certification Date: 11/06/2013
Installation Date: 11/07/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.71 V
Cooler Voltage = 1.70 V
Bias Voltage   = 80 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 4.436 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0317    0.0346
MIN(V)   0.0305    0.0335

FILTER INFO
Filter 1   0.034  Zero = true
Filter 2   0.613  Zero = true
Filter 3   0.225  Zero = true

CALIBRATION CHECK
Xq  = 0.104  0.08%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-16-100
Range	= 0.094 - 0.104
Average	= 0.096 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

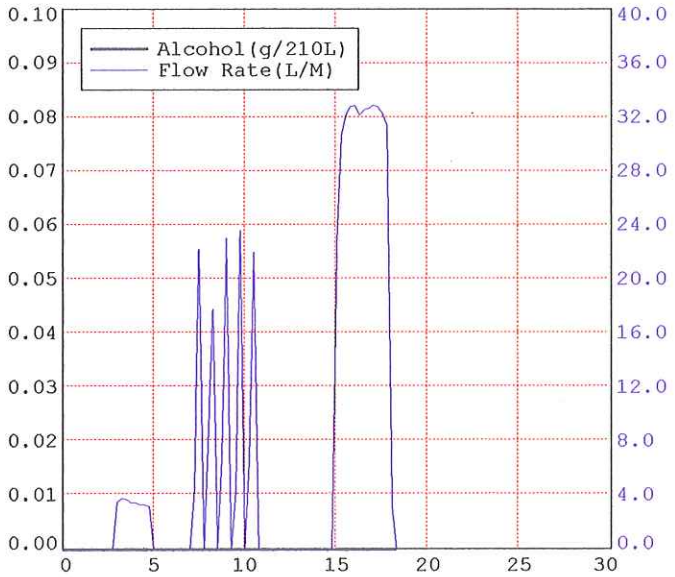

INSTALLATION PASSED

Performed by RCD **Date** 11/07/2013

Reviewed by **Date** 11/8/2013