INSTALLATION REPORT

DataMaster DMT: 100152
Location: Woodstock PD
Calibration Date: 10/28/2014
Certification Date: 10/28/2014
Installation Date: 10/29/2014
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.71 V
Cooler Voltage = 1.72 V
Bias Voltage   = 80 V
Chopper Freq   = 521 Hz

PUMP INFO
Flow Rate = 4.735 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1913    0.1955
MIN(V)   0.1894    0.1935

FILTER INFO
Filter 1   0.194  Zero = true
Filter 2   0.520  Zero = true
Filter 3   1.131  Zero = true

CALIBRATION CHECK
Xq  = 0.084  0.10%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-14-100
Range	= 0.094 - 0.104
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

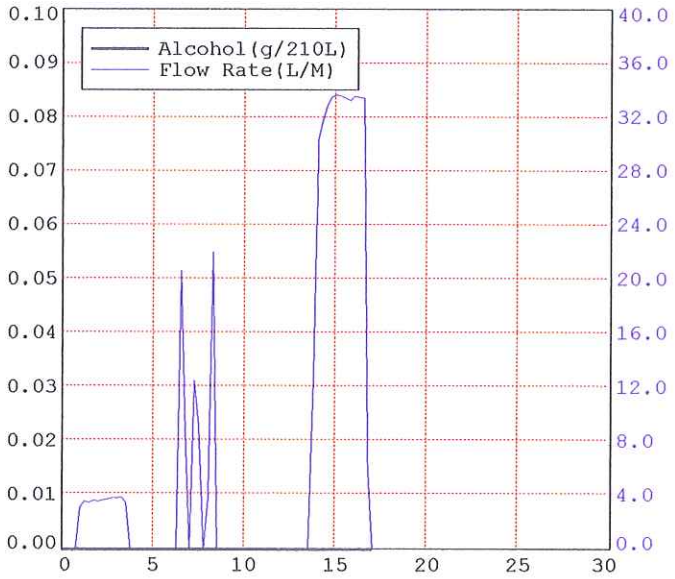

INSTALLATION PASSED

NIST Thermometer S/N 111814517 34.1°C RCD 10/29/14

Performed by RCD **Date** 10/29/2014

Reviewed by TLCA **Date** 10/30/2014