INSTALLATION REPORT

DataMaster DMT: 100132
Location: Williston VSP
Calibration Date: 12/14/2011
Certification Date: 12/14/2011
Installation Date: 12/21/2011
Installed by: AMANDA BOLDUC

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.57 V
Cooler Voltage = 1.65 V
Bias Voltage   = 80 V
Chopper Freq   = 540 Hz

PUMP INFO
Flow Rate = 5.727 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0148   -0.0112
MIN(V)   -0.0161   -0.0126

FILTER INFO
Filter 1  -0.011  Zero = true
Filter 2   0.869  Zero = true
Filter 3   0.068  Zero = true

CALIBRATION CHECK
Xq  = 0.090  0.48%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

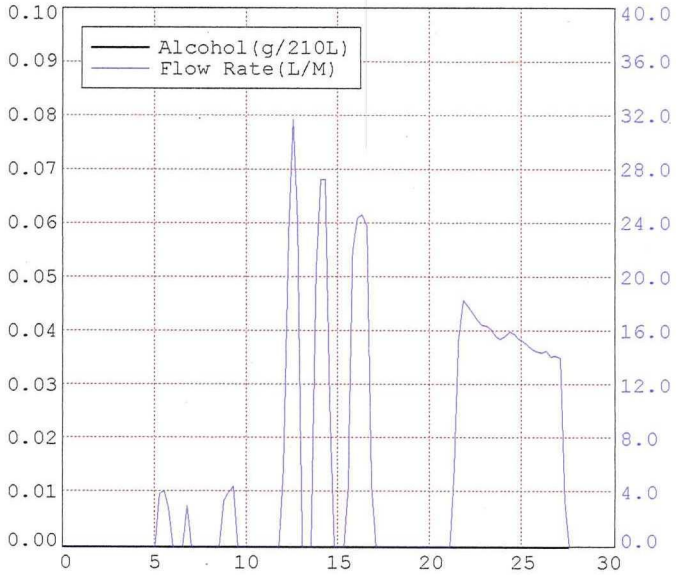

INSTALLATION PASSED

Rev. 12-22-11

Performed by _____ Date 12/21/2011

Reviewed by _____ Date 12/21/11