INSTALLATION REPORT

DataMaster DMT: 100132
Location: Williston VSP
Calibration Date: 12/14/2011
Certification Date: 12/14/2011
Installation Date: 05/31/2012
Installed by: AMANDA BOLDUC

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 47.6°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.57 V
Cooler Voltage = 1.65 V
Bias Voltage   = 80 V
Chopper Freq   = 544 Hz

PUMP INFO
Flow Rate = 5.810 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1081    0.1106
MIN(V)   0.1063    0.1085

FILTER INFO
Filter 1   0.110  Zero = true
Filter 2   0.973  Zero = true
Filter 3   0.180  Zero = true

CALIBRATION CHECK
Xq  = 0.090  0.39%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

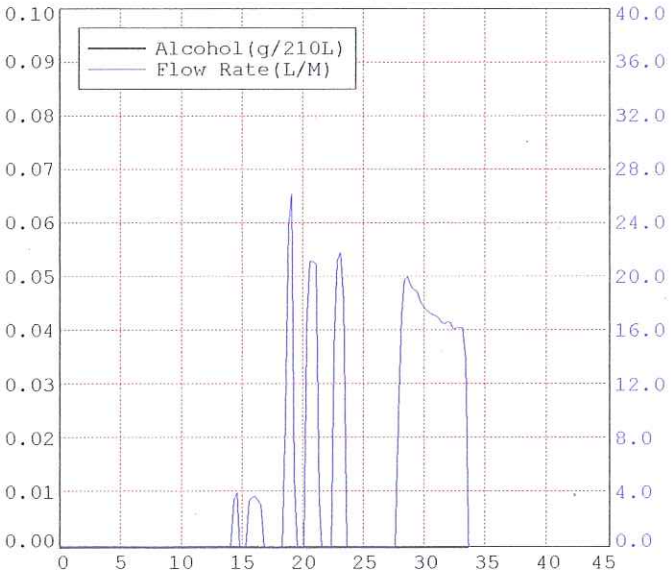

INSTALLATION PASSED

Performed by Date 05/31/2012

Reviewed by Date 6/7/2012