INSTALLATION REPORT

DataMaster DMT: 100134
Location: Morristown PD
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 02/09/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.66 V
Cooler Voltage = 1.66 V
Bias Voltage   = 80 V
Chopper Freq   = 523 Hz

PUMP INFO
Flow Rate = 5.635 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0778   -0.0736
MIN(V)   -0.0789   -0.0746

FILTER INFO
Filter 1  -0.073  Zero = true
Filter 2   0.473  Zero = true
Filter 3   0.604  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.52%
```

Accuracy and Precision Check

Concentration = 0.100 g/210L
Lot # = 12-51-100
Range = 0.095 - 0.105
Average = 0.099 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

No Base Radio at site 2/9/12
02/09/12
2-13-12

Sample Acceptance Test

Passed

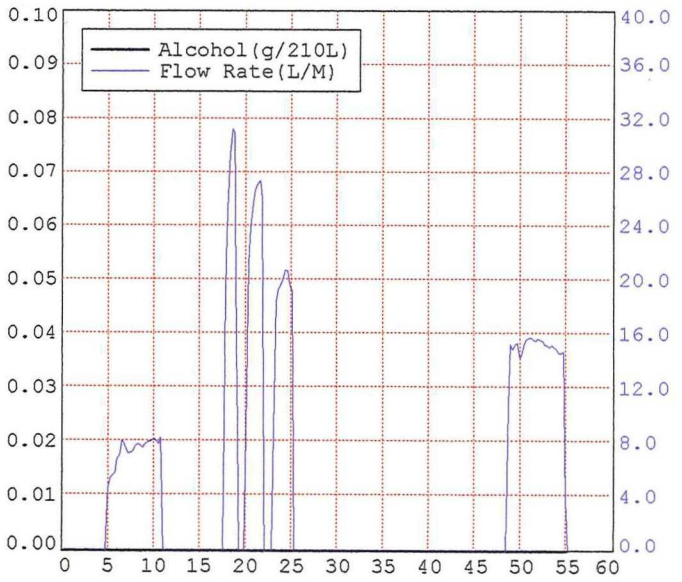

INSTALLATION PASSED

2/10/12
2-13-12

Performed by _____ Date 02/09/2012

Reviewed by _____ Date 02/09/12