INSTALLATION REPORT

DataMaster DMT: 100137
Location: GRAND ISLE COUNTY SO
Calibration Date: 09/28/2016
Certification Date: 09/28/2016
Installation Date: 09/29/2016
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.65 V
Cooler Voltage = 1.69 V
Bias Voltage   = 80 V
Chopper Freq   = 540 Hz

PUMP INFO
Flow Rate = 5.573 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1291    0.1329
MIN(V)   0.1274    0.1313

FILTER INFO
Filter 1   0.132  Zero = true
Filter 2   0.402  Zero = true
Filter 3   0.581  Zero = true

CALIBRATION CHECK
Xq  = 0.083  1.03%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 16-05-100
Range	= 0.094 - 0.104
Average	= 0.102 g/210L
Std Dev	= 0.0004

RF Detection Test

Passed

Sample Acceptance Test

Passed

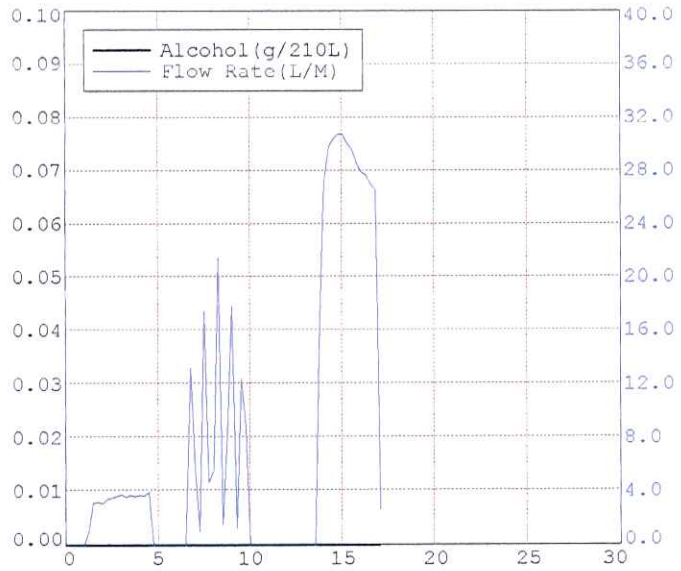

INSTALLATION PASSED

NIST Thermometer S/N 111814367 34.2°C
RCD 9/29/16

Performed by RCD Date 09/29/2016

Reviewed by AB Date 10/4/16