INSTALLATION REPORT

DataMaster DMT: 100139
Location: Bennington PD
Calibration Date: 09/26/2011
Certification Date: 09/28/2011
Installation Date: 10/11/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 33.7°C

SETTINGS
Lamp Voltage   = 1.80 V
Cooler Voltage = 1.69 V
Bias Voltage   = 80 V
Chopper Freq   = 532 Hz

PUMP INFO
Flow Rate = 6.384 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0915   -0.0882
MIN(V)   -0.0931   -0.0896

FILTER INFO
Filter 1  -0.090  Zero = true
Filter 2   0.265  Zero = true
Filter 3   0.898  Zero = true

CALIBRATION CHECK
Xq  = 0.082  0.21%
```

Accuracy and Precision Check

Concentration	= 0.102 g/210L
Lot #	= 12-13-100
Range	= 0.097 - 0.107
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

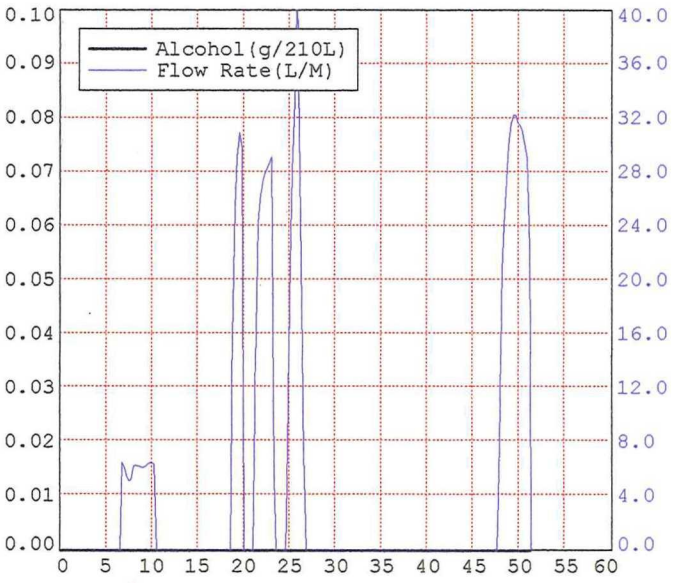

INSTALLATION PASSED

Performed by _____ Date 10/11/2011 10-12-11

Reviewed by _____ Date 10/11/11