INSTALLATION REPORT

DataMaster DMT: 100141
Location: VFL
Calibration Date: 01/30/2012
Certification Date: 01/31/2012
Installation Date: 06/10/2014
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 46.8°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage   = 81 V
Chopper Freq   = 533 Hz

PUMP INFO
Flow Rate = 6.021 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0762    0.0785
MIN(V)   0.0748    0.0772

FILTER INFO
Filter 1   0.078  Zero = true
Filter 2   0.388  Zero = true
Filter 3   0.671  Zero = true

CALIBRATION CHECK
Xq  = 0.081  1.06%
```

Accuracy and Precision Check

Concentration	= 0.097 g/210L
Lot #	= 14-02-100
Range	= 0.092 - 0.102
Average	= 0.096 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

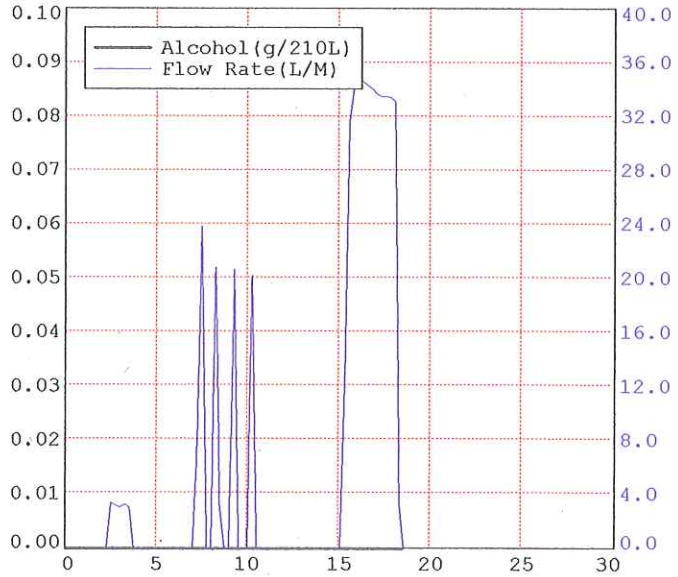

INSTALLATION PASSED

Performed by RCD **Date** 06/10/2014

Reviewed by **Date** 6/11/2014