

# INSTALLATION REPORT



DataMaster DMT: 100141  
Location: Windham County SO - Vernon  
Calibration Date: 01/30/2012  
Certification Date: 01/31/2012  
Installation Date: 05/28/2015  
Installed by: ROBERT DRISCOLL

## Default Options Loaded

### Diagnostic Results

VERSIONS  
DMT: 1.01  
PIC: 2.05  
Modem: 2.4  
Questions: 2.1

#### TEMPERATURES

Sample Chamber = 48.7°C  
Breath Tube = 44.4°C  
Digital Sim = 34.0°C

#### SETTINGS

Lamp Voltage = 1.73 V  
Cooler Voltage = 1.72 V  
Bias Voltage = 81 V  
Chopper Freq = 537 Hz

#### PUMP INFO

Flow Rate = 6.065 L/M

#### DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0722	0.0754
MIN (V)	0.0707	0.0740

#### FILTER INFO

Filter 1	0.074	Zero = true
Filter 2	0.381	Zero = true
Filter 3	0.655	Zero = true

#### CALIBRATION CHECK

Xq = 0.081 1.69%

### Accuracy and Precision Check


Concentration = 0.100 g/210L  
Lot # = 15-06-100  
Range = 0.095 - 0.105  
Average = 0.097 g/210L  
Std Dev = 0.0000

### RF Detection Test

Passed

### Sample Acceptance Test

Passed

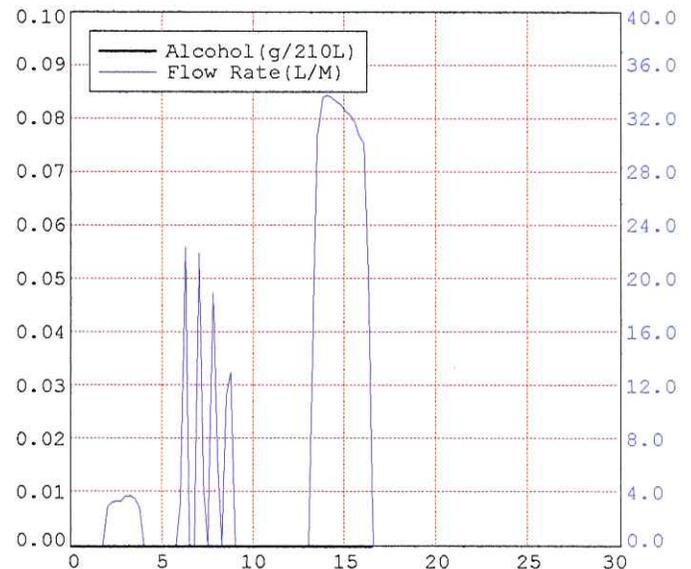

## INSTALLATION PASSED

*NIST Thermometer s/n 11814512 34.0°C RD 5/28/15*

Performed by *RD*

Date 05/28/2015

Reviewed by *RD*

Date 6/8/15

VERMONT FORENSIC LABORATORY

PO BOX 47  
 WATERBURY, VERMONT 05676-0047  
 TEL: 802-244-8788  
 FAX: 802-241-5557  
<http://vfl.vermont.gov>



**DataMaster DMT Site Evaluation Checklist**

Agency or Site Information

Name: LT MARK ANDERSON

Address: 567 GOVERNOR HUNT RD  
VERNON VT 05354

Phone: 802-254-6962

Fax: 802-258-2325

Personnel Information

Head of Site: LT MARK ANDERSON

Current DataMaster Supervisor (s):  
DFC CHRIS NORTON

Proposed DataMaster Supervisor(s):  
SAME

(Proposed) DataMaster DMT Environment

Limited Controlled Access:	<input checked="" type="radio"/>	N
Low Activity Area:	<input checked="" type="radio"/>	N
Unlimited Access by Other Law Enforcement Personnel	<input checked="" type="radio"/>	N
Access by VFL Technical Services	<input checked="" type="radio"/>	N
Air Conditioned	<input checked="" type="radio"/>	N
Room Temperature 65° - 85° F	<input checked="" type="radio"/>	N
Adequate Ventilation	<input checked="" type="radio"/>	N
Free of Cleaning Supplies	<input checked="" type="radio"/>	N
Clean	<input checked="" type="radio"/>	N

(Proposed) DataMaster DMT Connection(s)

Power:		
Min 15 Amp	<input checked="" type="radio"/>	N
Limited low power sharing:	<input checked="" type="radio"/>	N
Ethernet Available:	Y	<input checked="" type="radio"/>
Distance to Ethernet	_____	

(Proposed) DataMaster DMT Site Maintenance Agreement

Will notify VFL Alcohol Program staff of maintenance and supply needs promptly:	<input checked="" type="radio"/>	N
Will notify VFL Alcohol Program staff of changes in building conditions or moves promptly:	<input checked="" type="radio"/>	N
Will notify VFL Alcohol Program staff of relevant personnel changes at site promptly:	<input checked="" type="radio"/>	N

VFL Representative:	<u>Robert Dancell</u> Print Name	<u>[Signature]</u> Signature	<u>5/28/15</u> Date
Agency Representative:	<u>LT Mark Anderson</u> Print Name	<u>[Signature]</u> Signature	<u>5/28/15</u> Date