ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100148
Location: Berlin PD
Calibration Date: 11/09/2011
Certification Date: 11/14/2011
Installation Date: 12/08/2011
RPC Date: 02/02/2013
Supervisor Name: MARK A MONTEITH

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.64 V
Cooler Voltage = 1.69 V
Bias Voltage   = 80 V
Chopper Freq   = 538 Hz

PUMP INFO
Flow Rate = 5.833 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1701    0.1742
MIN(V)   0.1685    0.1728

FILTER INFO
Filter 1   0.173  Zero = true
Filter 2   0.517  Zero = true
Filter 3   0.372  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.00%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

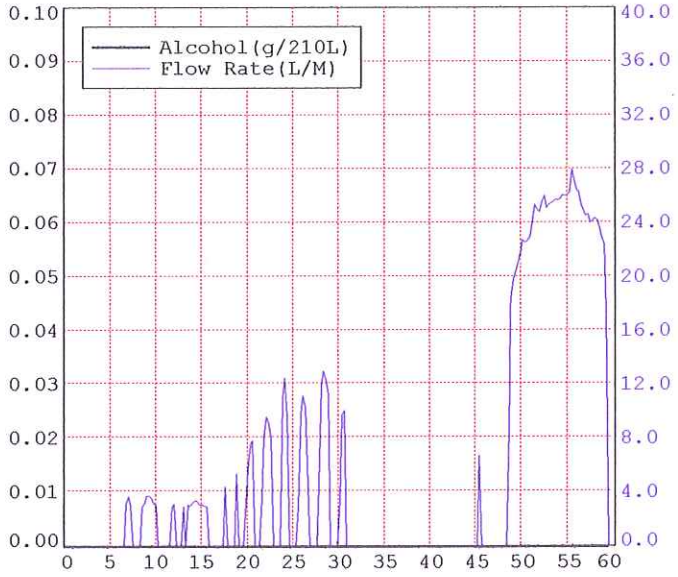

Performed by Mark Monteith **Date** 02/02/2013

Reviewed by [illegible] **Date** 2/8/13

2/11/2013