

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100148
Location: Berlin PD
Calibration Date: 11/09/2011
Certification Date: 11/14/2011
Installation Date: 12/08/2011
RPC Date: 06/27/2013
Supervisor Name: MARK A MONTEITH

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.64 V
Cooler Voltage = 1.69 V
Bias Voltage = 80 V
Chopper Freq = 540 Hz

PUMP INFO

Flow Rate = 5.845 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.2295	0.2321
MIN (V)	0.2278	0.2307

FILTER INFO

Filter 1	0.231	Zero = true
Filter 2	0.576	Zero = true
Filter 3	0.444	Zero = true

CALIBRATION CHECK

Xq = 0.085 1.57%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 1284100
Range	= 0.096 - 0.106
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

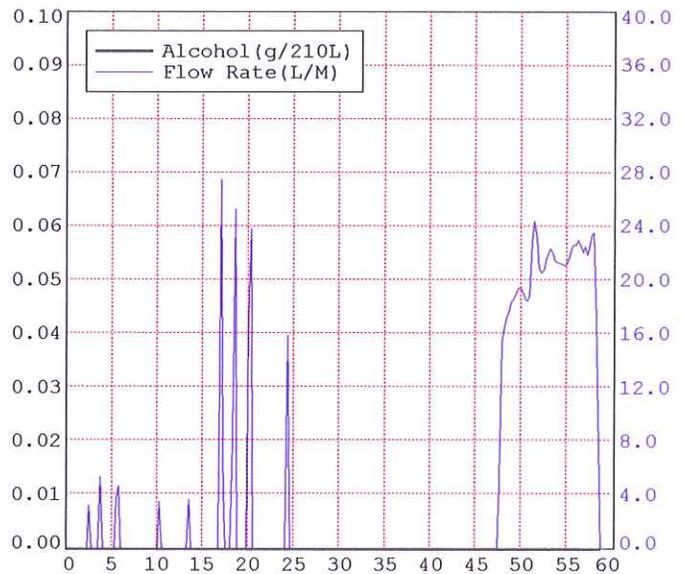

Performed by Mark Monteith

Date 06/27/2013

Reviewed by [Signature]

Date 8/7/13

DMT Serial Number #100148


Page 1 of 1

08/07/2013 12:00 PM

Page 1 of 8 rec

[Signature]
8/7/2013

ROUTINE PERFORMANCE CHECK REPORT

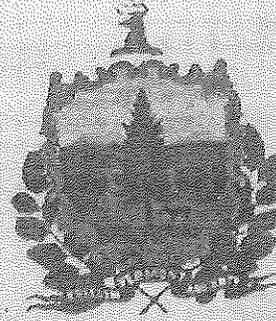

DataMaster DMT: 100148
Location: Berlin PD
Calibration Date: 11/09/2011
Certification Date: 11/14/2011
Installation Date: 12/08/2011
RPC Date: 06/27/2013
Supervisor Name: MARK A MONTEITH

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.64 V
Cooler Voltage = 1.69 V
Bias Voltage = 80 V
Chopper Freq. = 540 Hz

PUMP INFO

Flow Rate = 5.845 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.2295	0.2321
MIN (V)	0.2278	0.2307

FILTER INFO

Filter	Value	Zero
Filter 1	0.231	Zero = true
Filter 2	0.576	Zero = true
Filter 3	0.444	Zero = true

CALIBRATION CHECK

Xq = 0.085 1.57%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.101 g/210L
Lot # = 1284100
Range = 0.096 - 0.106
Average = 0.101 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

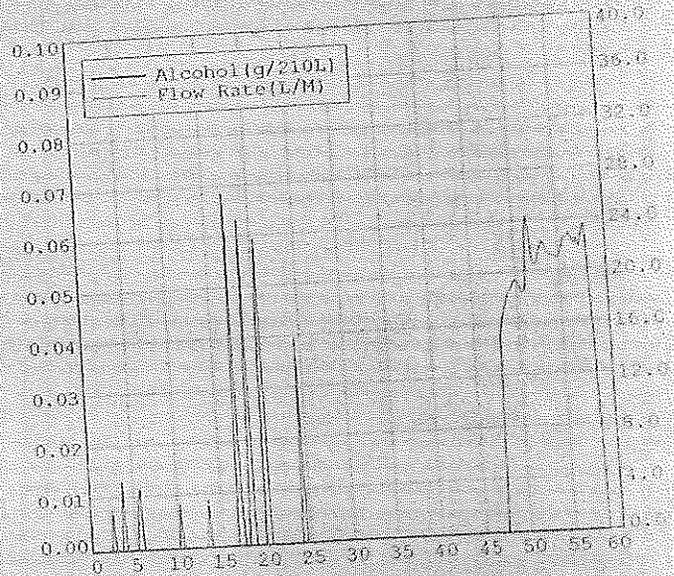

* requested color copy on 7/17/13

Performed by

Mark A Monteith

Date

06/27/2013

Reviewed by

[Signature]

Date

7/17/13

DMT Serial Number #100148

Page 1 of 1

06/27/2013 5:01 PM

2008 RCO

Driscoll, Rob

From: Monteith, Mark
Sent: Wednesday, July 17, 2013 12:26 PM
To: Driscoll, Rob
Subject: RE:

Will get the copies mailed, my scanner doesn't work well

sorry for the confusion

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: Driscoll, Rob
Sent: Wednesday, July 17, 2013 12:24 PM
To: Monteith, Mark
Subject: RE:

Mark,

I need a scanned copy or a copy mailed to me. The color photo does not suffice for our records. If you have any questions feel free to give me a call.

Thanks,
Rob

Robert Driscoll
Vermont Forensics Laboratory
Electronics Technician
Rob.Driscoll@state.vt.us
Desk: (802) 241-5817
Cell: (802) 585-0123

From: Monteith, Mark
Sent: Wednesday, July 17, 2013 12:22 PM
To: Driscoll, Rob
Subject: FW:

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: monteith82@gmail.com [monteith82@gmail.com]

Sent: Wednesday, July 17, 2013 11:54 AM

To: Monteith, Mark

Subject:

Sent from my Verizon Wireless 4G LTE DROID

Driscoll, Rob

From: Monteith, Mark
Sent: Tuesday, July 16, 2013 5:30 PM
To: Driscoll, Rob
Subject: RE: June RPC Overdue
Attachments: data 1.jpg; data 2.jpg; data 3.jpg; data 4.jpg

Rob

here are pics of the reports

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: Driscoll, Rob
Sent: Tuesday, July 16, 2013 2:30 PM
To: Monteith, Mark
Subject: RE: June RPC Overdue

Great! You can also scan me the RPC if you have a color scanner.

Thanks again,
Rob

From: Monteith, Mark
Sent: Tuesday, July 16, 2013 2:29 PM
To: Driscoll, Rob
Subject: RE: June RPC Overdue

yes I can, out on the rd, but will do by end of day

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: Driscoll, Rob
Sent: Tuesday, July 16, 2013 2:26 PM
To: Monteith, Mark
Subject: RE: June RPC Overdue

Mark,

Can you scan and send me the three logs (Breath Record History, Status Record History, and Log On Record History)...even if they are blank so that we can see what you are referring to.

Thanks,
Rob

From: Monteith, Mark
Sent: Tuesday, July 16, 2013 11:05 AM
To: Driscoll, Rob; Bassette, Chad
Subject: RE: June RPC Overdue

Rob, what we are having for an issue is when we print the user log we only get the log on and status sheet , the individuals who have signed on, dates, time ect do not print out on the form??

I don't know if you have any suggestions as I'm sure there should be entries printing on the forms.

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: Driscoll, Rob
Sent: Monday, July 15, 2013 9:08 AM
To: Monteith, Mark; Bassette, Chad
Subject: RE: June RPC Overdue

Chad or Mark,

Have you resolved your printer issues? If the instrument won't print, make sure that the printer is not in error (need paper/ink, etc), then reset the DataMaster (turn off for one minute then turn back on). I am looking for just a color copy of the June RPC. We need it to update our records and make sure the DMT is still in compliance with our standards. Also, the simulator solution must be placed in use before the expiration date, it does not actually expire if it is already in use before the expiration date. We will send you one more bottle as a backup. If you have any question feel free to give me a call.

Regards,
Rob

Robert Driscoll
Vermont Forensics Laboratory
Electronics Technician
Rob.Driscoll@state.vt.us
Desk: (802) 241-5817
Cell: (802) 585-0123

From: Monteith, Mark
Sent: Tuesday, July 09, 2013 11:42 AM
To: Bassette, Chad; Driscoll, Rob
Subject: RE: June RPC Overdue

Rob

The RPC was done, the paper work was not sent as we finished it after hours and we were unable to get the log in report to print, no sign ons were showing. I must have mis communicated with Chad as I thought he was going to contact your office to see if the issue could be figured out as well as order more solution as what we have in the instrument expires in September as dose the only other extra bottle that we have.

Sergeant Mark Monteith
Berlin Police Department
108 Shed Road
Berlin, VT 05602

From: Bassette, Chad
Sent: Monday, July 08, 2013 3:44 PM
To: Driscoll, Rob; Monteith, Mark
Subject: Re: June RPC Overdue

I was on vacation when Sgt. Monteith completed it. I will attach this to him and he is in tomorrow and will send it to you.

Thanks

Sent from my Verizon Wireless 4G LTE Smartphone

----- Reply message -----

From: "Driscoll, Rob" <Rob.Driscoll@state.vt.us>
To: "Bassette, Chad" <Chad.Bassette@state.vt.us>
Subject: June RPC Overdue
Date: Mon, Jul 8, 2013 3:06 PM

Chad,

Can you please send me a copy of the RPC. I don't see it in our records anywhere.

Thanks,
Rob

From: Bassette, Chad
Sent: Monday, July 08, 2013 3:01 PM
To: Driscoll, Rob
Subject: Re: June RPC Overdue

We did do it

Sent from my Verizon Wireless 4G LTE Smartphone

----- Reply message -----

From: "Driscoll, Rob" <Rob.Driscoll@state.vt.us>
To: "Campbell, Greg" <Greg.Campbell@state.vt.us>, "Ambroz, Todd" <Todd.Ambroz@state.vt.us>, "Ravelin, Paul" <Paul.Ravelin@state.vt.us>, "Reeve, Michael" <Michael.Reeve@state.vt.us>, "Shelp, Benjamin" <Benjamin.Shelp@state.vt.us>, "Skochin, Kerry" <Kerry.Skochin@state.vt.us>, "Leonard, Anthony" <Anthony.Leonard@state.vt.us>, "Norton, Christopher" <Christopher.Norton@state.vt.us>, "Bassette, Chad" <Chad.Bassette@state.vt.us>, "Monteith, Mark" <Mark.Monteith@state.vt.us>, "Spacapan, Patricia" <Patricia.Spacapan@state.vt.us>, "Roy, James" <James.Roy@state.vt.us>

"Lehneman, Jack" <Jack.Lehneman@state.vt.us>, "Howard, Joel" <Joel.Howard@state.vt.us>, "Noblet, Jason" <Jason.Noblet@state.vt.us>, "Sly, John" <John.Sly@state.vt.us>, "Noyes, Jeffrey" <Jeffrey.Noyes@state.vt.us>, "Adams, Jonathan" <Jonathan.Adams@state.vt.us>, "Rainault, Gil" <Gil.Rainault@state.vt.us>, "Deslauriers, Katherine" <Katherine.Deslauriers@state.vt.us>, "Kevin Emilio" <kemilio@middleburypolice.org>, "Christopher Mason" <cmason@middleburypolice.org>, "Jason Covey" <jcovey@middleburypolice.org>
Cc: "Bolduc, Amanda" <Amanda.Bolduc@state.vt.us>, "Conti, Trisha" <Trisha.Conti@state.vt.us>
Subject: June RPC Overdue
Date: Mon, Jul 8, 2013 2:30 PM

Our records indicate that you have not yet performed the June RPC for your DataMaster DMT. As of July 1, your DMT has been removed from service until such time as a passing RPC is completed. Please submit a color copy of your results to us via e-mail or mail as soon as possible.

If you have any questions, please reach out to me or Trisha Conti (trisha.conti@state.vt.us or 241-5436).

Regards,
Rob

Robert Driscoll
Vermont Forensics Laboratory
Electronics Technician
Rob.Driscoll@state.vt.us
Desk: (802) 241-5817
Cell: (802) 585-0123