

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100149
 Location: Barre City PD
 Calibration Date: 10/12/2011
 Certification Date: 10/13/2011
 Installation Date: 12/06/2011
 RPC Date: 02/02/2013
 Supervisor Name: TROY S KIRKPATRICK

Diagnostic Results

VERSIONS
 DMT: 1.01
 PIC: 2.06
 Modem: 2.4
 Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
 Breath Tube = 46.0°C
 Digital Sim = 33.8°C

SETTINGS

Lamp Voltage = 1.78 V
 Cooler Voltage = 1.61 V
 Bias Voltage = 80 V
 Chopper Freq = 535 Hz

PUMP INFO

Flow Rate = 5.631 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.3276	0.3313
MIN (V)	0.3262	0.3297

FILTER INFO

Filter	Value	Zero
Filter 1	0.330	Zero = true
Filter 2	0.603	Zero = true
Filter 3	0.827	Zero = true

CALIBRATION CHECK

Xq = 0.080 0.00%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.101 g/210L
 Lot # = 12-87-100
 Range = 0.096 - 0.106
 Average = 0.099 g/210L
 Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

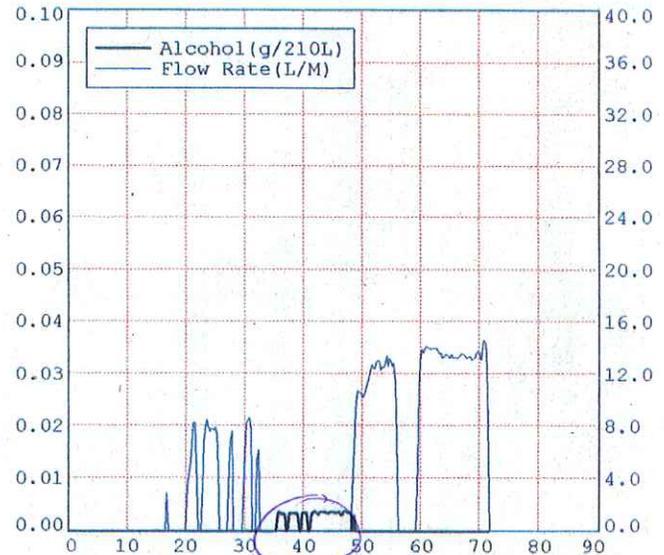

See attached email regarding sample acceptance. RCD 2/6/13

Performed by *T. S. Kirkpatrick*

Date 02/02/2013

Reviewed by *T. S. Kirkpatrick*

Date 2/6/13

DMT Serial Number #100149

T. S. Kirkpatrick
 2/11/2013



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 100149
Location: Barre City PD
Certification Date: 10/13/2011
Installation Date: 12/06/2011


Date: 02/05/2013
Time: 08:13:29

SUBJECT NAME:
RPC RPC TEST
DOB: 01/01/1989 AGE: 24
GENDER: M

TEST OPERATOR NAME:
ANDREW W MARCEAU
AGENCY: barre city

BLANK TEST	0.000	08:14
CALIBRATION CHECK	PASSED	08:14
SIMULATOR VAPOR 33.8°C	0.098	08:14
SUBJECT SAMPLE (Vol=2.9L)	0.000	08:15
BLANK TEST	0.000	08:16

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.101
Sim. Vapor Range 0.096 - 0.106
Lot #: 12-87-100

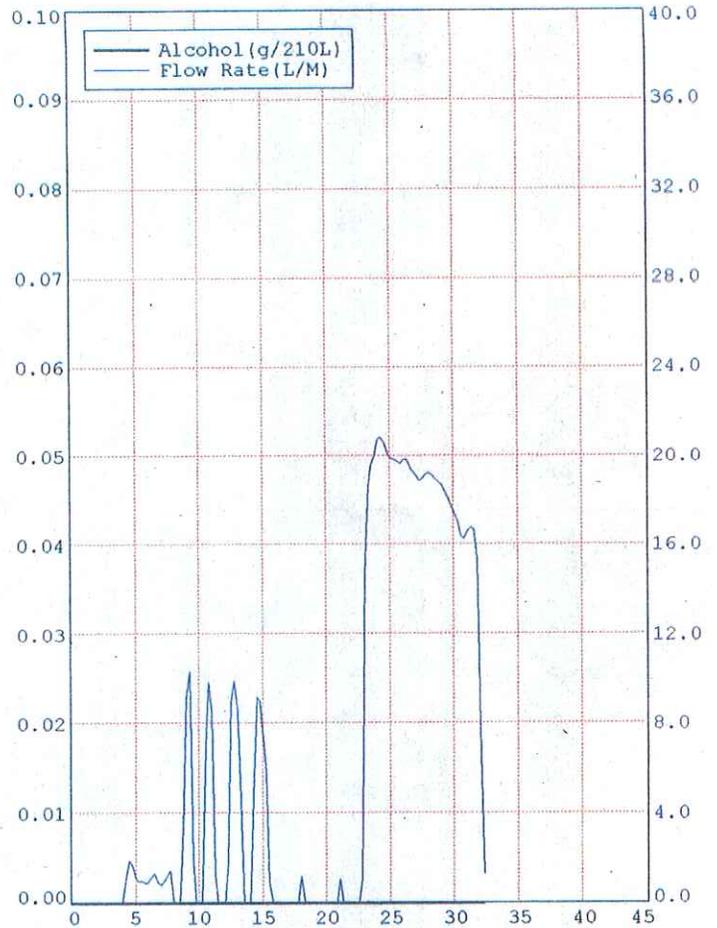

Driscoll, Rob

From: Marceau, Andrew
Sent: Tuesday, February 05, 2013 8:33 AM
To: Driscoll, Rob
Subject: RE: February RPC
Attachments: RPC Check-in.pdf

Rob,

Attached is the Check-in test

Andy

From: Driscoll, Rob
Sent: Monday, February 04, 2013 11:05 AM
To: Marceau, Andrew
Subject: RE: February RPC

Andy,

I received your February RPC, but noticed there is an alcohol "blip" in the sample acceptance. Can you please perform a "Check-In" and include each of the four breath samples (shallow, intermittent, suck-back, and alcohol free breath sample). I will need a color copy of the check-in to pass the RPC.

Thanks,
Rob

From: Marceau, Andrew
Sent: Monday, February 04, 2013 10:58 AM
To: Driscoll, Rob
Subject: RE: February RPC

Sorry, forgot to attach

Andy

From: Driscoll, Rob
Sent: Monday, February 04, 2013 10:24 AM
To: Marceau, Andrew
Subject: RE: February RPC

Andy,

I'm not seeing the attachment?

Thanks,
Rob

From: Marceau, Andrew
Sent: Monday, February 04, 2013 10:21 AM
To: Driscoll, Rob
Subject: RE: February RPC

Attached is the RPC

Andy

Andrew W. Marceau
Deputy Chief of Police
Barre City Police Department
15 Fourth Street
Barre, VT 05641
802-476-6613

andrew.marceau@state.vt.us **** Please Note New Email Address ****

From: Driscoll, Rob
Sent: Wednesday, January 30, 2013 11:16 AM
To: Abell, Dustin; Adams, Jonathan; Allen, Blake; Allen, Ray; Ambroz, Todd; Bassette, Chad; Bennett, Daniel F; Benoit, Richard; Bickford, Mark; Bohnyak, William; Butterfield, David; Campbell, Greg; Carignan, Mark; Chad Bean; Christopher Mason; Cleary, Lester; Clifford, Eric; Cochran, Aaron; Cota, Drew; Crowe, Thomas; Cushing, Blake; Denault, Mark; Derrick Kendrew; Deslauriers, Katherine; Dominic Brodeur; Draper, Sarah; DuPont, Tom; Dwayne Mellis; Dziobek, James; Eggum, David; Ellis, Holly; Emery, Chad; Erica Moore; Evans, Jeremy; Gauld, Bruce; Gene Martin (Bradford PD); Gero, Michael; Gibbs, Kevin; Gilbert, Donald; Greenslet, Patrick; Hall, Michael L; Hanson, William; Hebert, MaryBeth; Hebert, Richard; Herbes, Cassandra; Howard, Joel; James Goslin; James Mills; Jason Covey; John Dunn; Jollymore, Eric; Jones, Christopher; Keefe, Michael; Kevin Emilio; King, Peter; King, Richard; Kinney, Tyson; Kipnes, Ethan; Kirkpatrick, Robert; Kirkpatrick, Troy; Knight, David; LaFlam, Jody; LaFountain, Gordon; Lauzon, Chris; Lavoie, Michael; Lehneman, Jack; Leonard, Anthony; Loomis, Seth; Lynch, James; Marceau, Andrew; Matt Collins; Maurice, Crista; Mayer, Nick; McClure, Bruce; McGuire, Howard; Meyer, Bret; Monteith, Mark; Moore, Holly; Morgan Lawton; Moulton, Charles; Newton, Brent; Noblet, Jason; Nokes, Jason; Norton, Christopher; Noyes, Jeffrey; O'Donnell, Hugh; O'Keefe, Christopher; Paul Fabiani; Perkins, Robert; Plante, Andrew; Poulin, Marc; Quesnel, Christopher; Rainault, Gil; Ravelin, Paul; Reeve, Michael; Robert Kissinger; Robinson, Dustin; Roy, James; Sarah Superneau; Satterfield, Charles; Simpson, Tom; Skochin, Kerry; Sly, John; Spacapan, Patricia; Spaulding, Frank E; Stearns, Steven; Steere, Daniel; Steeves, Matthew; Stephen Dunning; Stephen Nolan; Sweeny, Jay; Taylor, Stephanie; Tienken, Derrick; Vail, Braedon; Walker, Kyle; Watson, Christian; Welch, Michael; Werner, Rich; White, David; Whitehead, Charles; Whitney, Patricia; William Austin; Winn, Charles; Witherbee, Penny; Zorn, Jacob
Cc: Conti, Trisha; Bolduc, Amanda
Subject: February RPC

DMT Supervisors,

I just wanted to send a reminder that your February RPC will be due by the end of next month. Please send a color copy to the Vermont Forensic Lab and keep the other for your records. If you need any DataMaster supplies just send me a note or fax a "supplies request form" to the number below. If anyone on this distribution list is no longer a DMT supervisor, please let me know so that I can update my records. For any questions or concerns feel free to contact me.

Regards,
Rob

Robert Driscoll
Electronics Technician
Vermont Forensic Laboratory
103 South Main Street
Waterbury, VT 05671-2101
(802) 241-5817 (desk)
Fax (802) 241-5557