ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100149
Location: Barre City PD
Calibration Date: 06/25/2014
Certification Date: 06/30/2014
Installation Date: 06/30/2014
RPC Date: 06/12/2015
Supervisor Name: JUSTIN L PICKEL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 43.8°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.81 V
Cooler Voltage = 1.81 V
Bias Voltage   = 80 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 5.666 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.4051    0.4079
MIN(V)   0.4039    0.4069

FILTER INFO
Filter 1   0.407  Zero = true
Filter 2   0.683  Zero = true
Filter 3   0.907  Zero = true

CALIBRATION CHECK
Xq  = 0.082  1.07%
```

Routine Performance Check Passed

Accuracy and Precision Check

TV = 0.098

Concentration	= 0.093 g/210L
Lot #	= 15-01-100
Range	= 0.088 - 0.098
Average	= 0.096 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

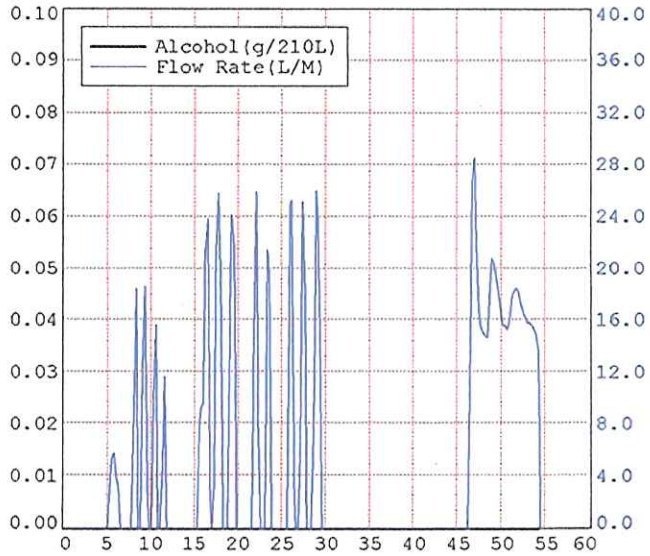

Called 6/16/15, DMT out of service until correct target can be entered AB

Performed by _____ Date 06/12/2015

Reviewed by _____ Date 6/22/15

SOLUTION CHANGE

DataMaster DMT: 100149
Location: Barre City PD
Date: 06/18/2015
Performed by: JUSTIN L PICKEL

Accuracy and Precision Check

Concentration	= 0.098 g/210L
Lot #	= 15-01-100
Range	= 0.093 - 0.103
Average	= 0.095 g/210L
Std Dev	= 0.0000

Simulator Temperature: 34°C

Performed by _____ Date 06/18/2015

2 JP

DUI SUBJECT TEST

STATE OF VERMONT

DataMater DMT: 100149
Location: Barre City PD
Certification Date: 06/30/2014
Installation Date: 06/30/2014

Date: 06/12/2015
Time: 19:32:38

SUBJECT NAME:
[redacted]
DOB: [redacted] AGE: [redacted]
GENDER: F
LICENSE #: [redacted]

CASE #: 15BA03612
TIME OF OPERATION: 18:30
LOCATION OF INCIDENT:
SUMMER STREET
TOWN: BARRE(CITY)
COUNTY: WASHINGTON

TEST OPERATOR NAME:
STEVEN D ROUNDS
AGENCY: BARRE CITY PD

Obs. Period Start:		19:00
Obs. Restart: belched		19:15
BLANK TEST	0.000	19:33
CALIBRATION CHECK	PASSED	19:33
SIMULATOR VAPOR 33.9°C	0.096	19:34
BLANK TEST	0.000	19:34
SUBJECT SAMPLE (Vol=4.1L)	0.230	19:35
BLANK TEST	0.000	19:36
CALIBRATION CHECK	PASSED	19:36
SIMULATOR VAPOR 34.0°C	0.093	19:37
BLANK TEST	0.000	19:37
SUBJECT SAMPLE (Vol=3.9L)	0.235	19:38

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.093
Sim. Vapor Range 0.088 - 0.098
Lot #: 15-01-100

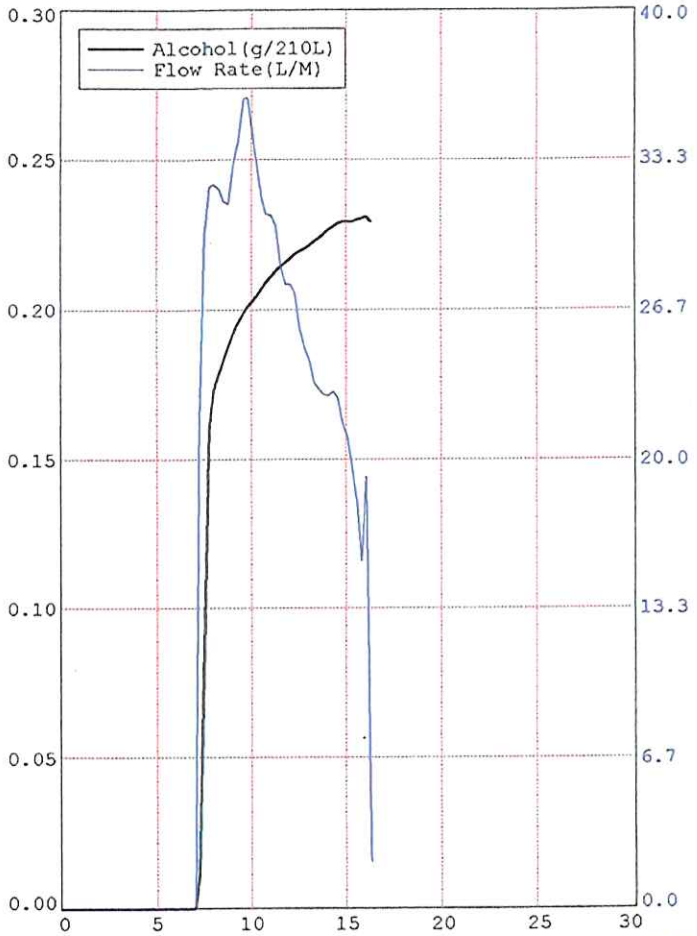

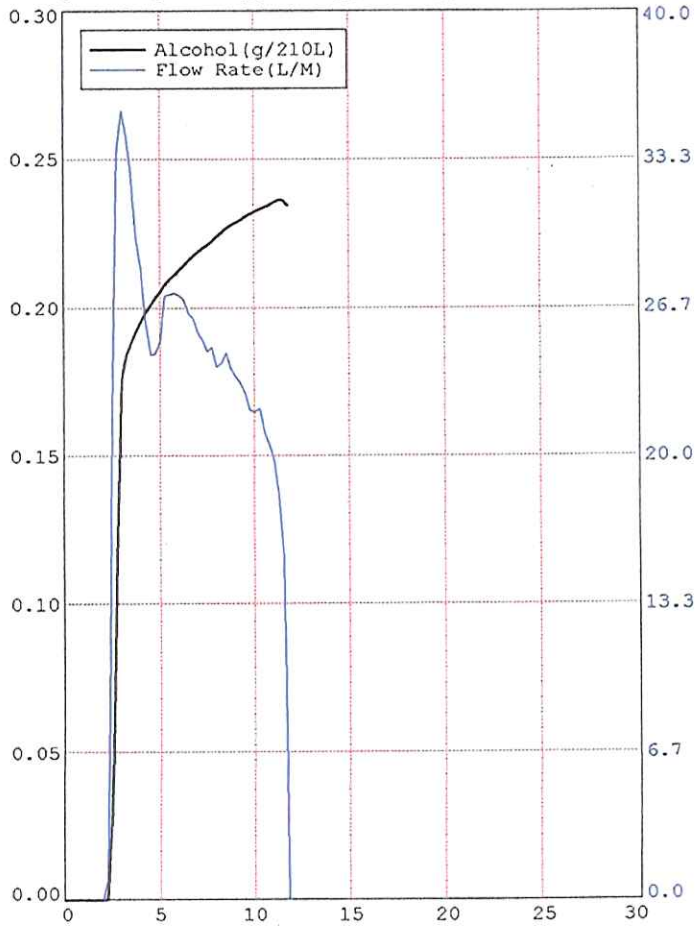

3 AB

Bolduc, Amanda

From: Pickel, Justin
Sent: Thursday, June 18, 2015 3:10 PM
To: Bolduc, Amanda
Subject: Data Master report
Attachments: DOC061815-06182015145311.pdf

Amanda

Attached is the solution change report and the DUI report from the 6/12/15 DUI arrest that Officer Rounds had.

Could you also send me some new solution I am out.

Any other questions please let me know.

Officer Justin Pickel
Barre City Police Dept.
802-476-6613

4 AB