INSTALLATION REPORT

DataMaster DMT: 100152
Location: Woodstock PD
Calibration Date: 03/07/2012
Certification Date: 03/07/2012
Installation Date: 03/08/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.71 V
Cooler Voltage = 1.72 V
Bias Voltage = 81 V
Chopper Freq = 538 Hz

PUMP INFO
Flow Rate = 5.470 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.1346	0.1382
MIN(V)	0.1331	0.1364

FILTER INFO
Filter 1 0.136 Zero = true
Filter 2 0.473 Zero = true
Filter 3 1.068 Zero = true

CALIBRATION CHECK
Xq = 0.080 1.87%

Accuracy and Precision Check

Concentration = 0.100 g/210L
Lot # = 12-58-100
Range = 0.095 - 0.105
Average = 0.098 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

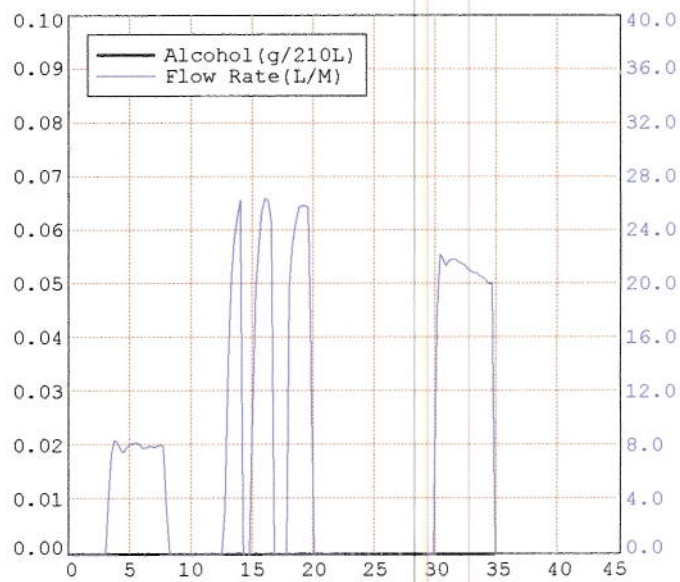

INSTALLATION PASSED

Performed by _____ Date 03/08/2012

Reviewed by _____ Date 3/19/12

TRC 3/27/2012