ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 100152
Location: Woodstock PD
Calibration Date: 03/07/2012
Certification Date: 03/07/2012
Installation Date: 03/08/2012
APM Date: 07/18/2013
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.71 V
Cooler Voltage = 1.72 V
Bias Voltage   = 81 V
Chopper Freq   = 557 Hz

PUMP INFO
Flow Rate = 5.604 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2669    0.2703
MIN(V)   0.2648    0.2685

FILTER INFO
Filter 1   0.269  Zero = true
Filter 2   0.591  Zero = true
Filter 3   1.203  Zero = true

CALIBRATION CHECK
Xq  = 0.080  0.99%
```

Simulator Vapor Test

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Simulator Vapor	= 0.096 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

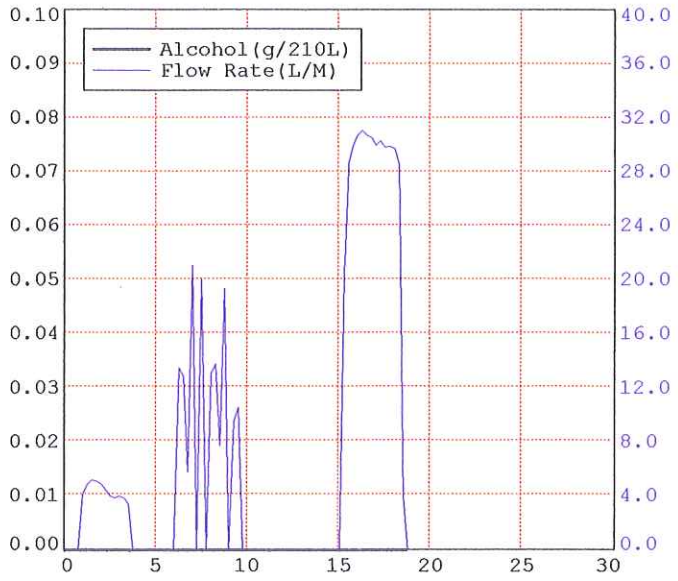

APM PASSED

NIST Thermometer S/N 111814522 33.9°C
RCD 7/18/13

Performed by RCD **Date** 07/18/2013

Reviewed by **Date** 7/22/2013