INSTALLATION REPORT

DataMaster DMT: 100153
Location: Brattleboro PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/02/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 48.0°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.78 V
Cooler Voltage = 1.84 V
Bias Voltage   = 80 V
Chopper Freq   = 530 Hz

PUMP INFO
Flow Rate = 5.533 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0441    0.0470
MIN(V)   0.0427    0.0449

FILTER INFO
Filter 1   0.045  Zero = true
Filter 2   0.281  Zero = true
Filter 3   0.650  Zero = true

CALIBRATION CHECK
Xq  = 0.076  0.58%
```

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 11-41-100
Range	= 0.096 - 0.106
Average	= 0.103 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

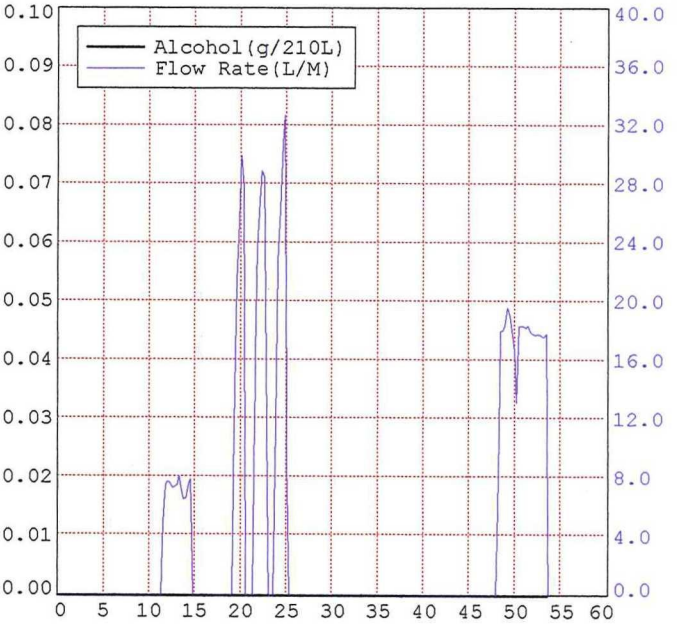

INSTALLATION PASSED

Performed by _____ Date 09/02/2011

Reviewed by _____ Date 9-2-11