ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100153
Location: Brattleboro PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/02/2011
RPC Date: 02/01/2015
Supervisor Name: ADAM S BELVILLE

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 41.3°C
Digital Sim    = 34.2°C

SETTINGS
Lamp Voltage   = 1.78 V
Cooler Voltage = 1.84 V
Bias Voltage   = 80 V
Chopper Freq   = 532 Hz

PUMP INFO
Flow Rate = 5.762 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.7583    0.7620
MIN(V)   0.7565    0.7600

FILTER INFO
Filter 1   0.760   Zero = true
Filter 2   0.961   Zero = true
Filter 3   1.241   Zero = true

CALIBRATION CHECK
Xq  = 0.076  0.58%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-15-100
Range	= 0.094 - 0.104
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

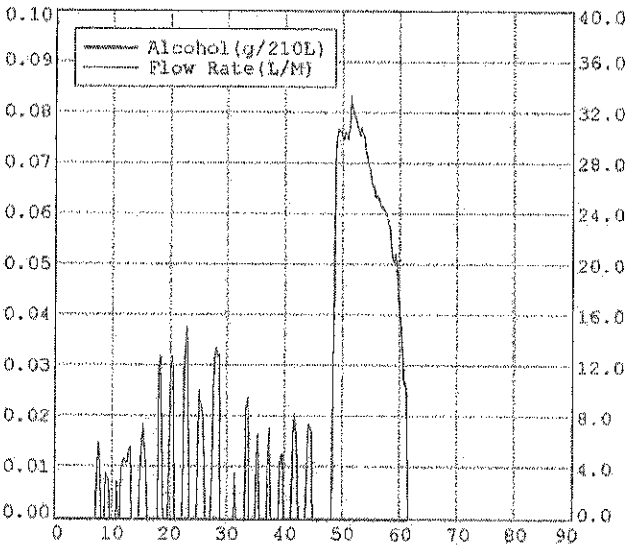

Performed by _____ Date 02/01/2015

Reviewed by _____ Date _____

DIAGNOSTIC RESULT

DataMaster DMT: 100153
Location: Brattleboro PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/02/2011
Test Date: 02/03/2015
Test Time: 21:52:18

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 40.8°C
Digital Sim = 34.1°C

SETTINGS
Lamp Voltage = 1.78 V
Cooler Voltage = 1.84 V
Bias Voltage = 80 V
Chopper Freq = 533 Hz

PUMP INFO
Flow Rate = 5.805 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.3587	0.3638
MIN(V)	0.3575	0.3626

FILTER INFO
Filter 1 0.363 Zero = true
Filter 2 0.586 Zero = true
Filter 3 0.890 Zero = true

CALIBRATION CHECK
Xq = 0.075 0.35%

DATAMASTER DMT MAINTENANCE LOG

Brattleboro Police
Department/Agency

100153
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
1/23/15	Screen frozen - turned power off and restarted [For RPC or Simulator Solution Change Place Label Here]	P. Withington M1239
2-1-15	[For RPC or Simulator Solution Change Place Label Here] DataMaster Simulator Solution Lot # 14-15-100 EtOHaq Conc: 0.099 g/210L Range: 0.094 - 0.104 Preparation Date: 12/9/2014 Expires: 12/9/2015 OPENED: 2-1-15 AB M1219	SGT. Adam Belville AB M1219
Sent to SA 2-2-15	RPC - Adam Belville 2-1-15	
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011

Status Record History

Status Date	Status Time	Test Type	Status Message
02/05/2015	03:34:32	DUI Subject Record	RESPONSE TIMEOUT

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
02/05/2015	03:29:11	BRATTLEBORO PD	ADAM S BELVILLE	0.122		0.098		RESPONSE TIMEOUT
02/05/2015	03:36:29	BRATTLEBORO PD	ADAM S BELVILLE	0.119		0.098		
02/17/2015	01:20:09	BRATTLEBORO PD	COLBY KERYLOW	REFUSED		0.096		
02/23/2015	00:25:48	BRATTLEBORO PD	JASON HAMILTONM	0.197		0.097		