

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100156
Location: FAIR HAVEN PD / Rutland VSP
Calibration Date: 07/16/2015
Certification Date: 07/16/2015
Installation Date: 07/17/2015
RPC Date: 10/23/2015
Supervisor Name: DALE H KERBER

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 46.0°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.96 V
Cooler Voltage = 1.89 V
Bias Voltage = 80 V
Chopper Freq = 539 Hz

PUMP INFO

Flow Rate = 5.974 L/M

DETECTOR INFO

PUMP ON OFF
MAX(V) -0.0049 -0.0014
MIN(V) -0.0079 -0.0045

FILTER INFO

Filter 1 -0.003 Zero = true
Filter 2 0.130 Zero = true
Filter 3 1.113 Zero = true

CALIBRATION CHECK

Xq = 0.086 0.00%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 15-09-100
Range = 0.094 - 0.104
Average = 0.101 g/210L
Std Dev = 0.0004

RF Detection Test

Passed

Sample Acceptance Test

Passed

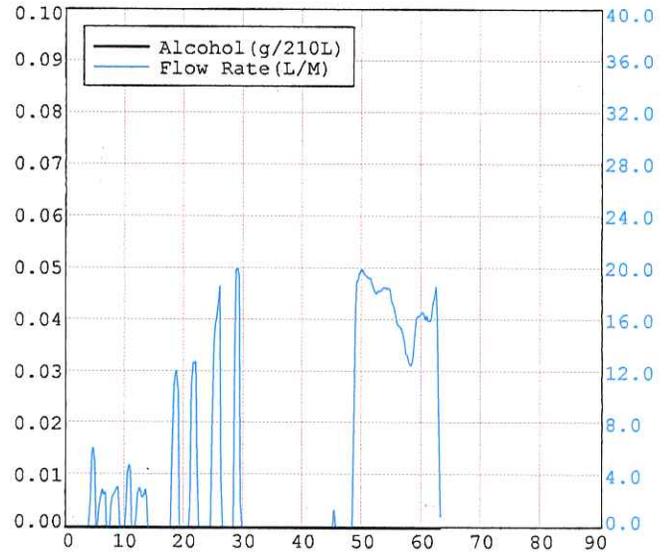

Performed by

Dale Kerber

Date 10/23/2015

Reviewed by

[Signature]

Date 10/26/15

[Signature]
10/27/15

DMT Serial Number #100156

Page 1 of 1

10/23/2015 9:57 PM

Page 1 of 3 RD

Driscoll, Rob

From: Driscoll, Rob
Sent: Monday, October 26, 2015 8:41 AM
To: Kerber, Dale
Subject: RE: Message from "RNP0026732353DE"

Dale,

It sounds like you may have keyed your mic too long during the RFI detection test. If you don't do just a quick key of the mic, the RF is detected again after the rf test and will abort the remainder of the RPC. I will ask Marcella to send out your supplies.

Regards,
Rob

Robert Driscoll
Vermont Forensics Laboratory
45 State Drive
Waterbury, VT 05671
Electronics Technician
Rob.Driscoll@Vermont.gov
Desk: (802) 241-5817
Cell: (802) 585-0123

-----Original Message-----

From: Kerber, Dale
Sent: Friday, October 23, 2015 10:08 PM
To: Driscoll, Rob
Subject: FW: Message from "RNP0026732353DE"

Rob, you can ignore my phone call from Friday night. I did get it to work, however after I ran through the entire process, instead of getting the message asking if everything passed, I got an Abort prompt, so I ran through another RPC and everything again passed but this time I got the correct message. Just letting you know.

Who do I contact for more mouthpieces? I also used the last Simulator Solution we have here as well,

Dale Kerber
Sergeant, Fair Haven Police Department
3 North Park Place,
Fair Haven, VT 05743
PH: (802)265-7839
Cell: (802)558-2518

From: [Fair Haven Outpost Copier@dps.state.vt.us](mailto:Fair_Haven_Outpost_Copier@dps.state.vt.us) [Fair_Haven_Outpost_Copier@dps.state.vt.us]
Sent: Friday, October 23, 2015 10:19 PM

