

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 09/12/2012
RPC Date: 11/01/2015
Supervisor Name: JACK B LEHNEMAN

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 44.7°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 555 Hz

PUMP INFO

Flow Rate = 4.356 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0925	0.0955
MIN(V)	0.0909	0.0937

FILTER INFO

Filter	Value	Zero
Filter 1	0.095	true
Filter 2	0.392	true
Filter 3	1.469	true

CALIBRATION CHECK

Xq = 0.093 1.01%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 15-12-100
Range = 0.094 - 0.104
Average = 0.097 g/210L
Std Dev = 0.0004

RF Detection Test

Passed

Sample Acceptance Test

Passed

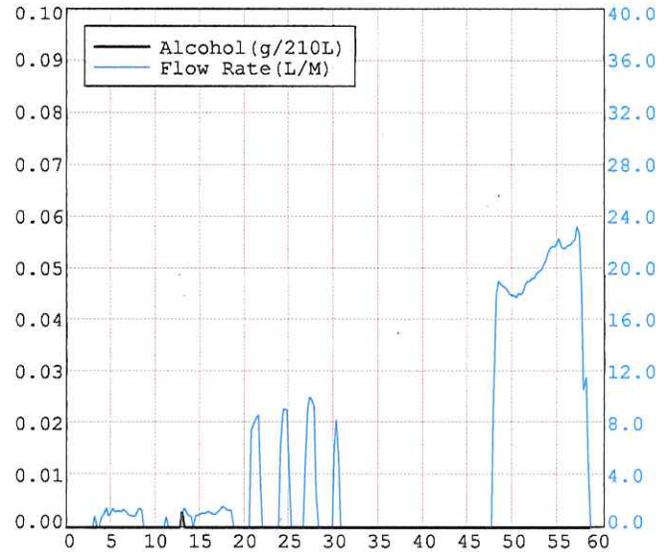

See attached "check-in" for passing sample acceptance R02 n13/15

Performed by

Jack Bell

Date

11/01/2015

Reviewed by

JBL

Date

n13/15

JBL
11/4/15

DMT Serial Number #100157

Page 1 of 1

11/01/2015 9:23 AM

Driscoll, Rob

From: Driscoll, Rob
Sent: Monday, November 02, 2015 10:32 AM
To: 'Ptl. Jack Lehneman'
Subject: RE: CPD October 2015 RPC

Jack,

After just looking at your RPC I noticed there was a "blip" in the alcohol line during your sample acceptance. Can you do a "check-in" using TEST, TEST for the subject name, with all four breaths (shallow, intermittent, gentle suck back, and 1.5 alcohol free sample)? Sorry, but that is not a passing sample anytime there is any movement of the alcohol line (the black line).

Thanks,
Rob

From: Ptl. Jack Lehneman [<mailto:jack.lehneman@colchesterpdvt.org>]
Sent: Monday, November 02, 2015 10:29 AM
To: Driscoll, Rob
Subject: Re: CPD October 2015 RPC

Thanks. I will send the empty bottles back on Wednesday.

Jack

Sent from my Verizon Wireless 4G LTE DROID

"Driscoll, Rob" <Rob.Driscoll@vermont.gov> wrote:

Jack,

I will send you two spare bottles and I'll just drop one at Winooski on my way home.

Thanks,
Rob

From: Ptl. Jack Lehneman [<mailto:jack.lehneman@colchesterpdvt.org>]
Sent: Sunday, November 01, 2015 9:37 AM
To: Driscoll, Rob
Cc: Ptl. Christopher Jones; Ptl. Derrick Kendrew; Sgt. James Roy
Subject: CPD October 2015 RPC

Rob,

I performed the RPC this morning and it is attached. I had to borrow a bottle of solution from Winooski PD because we were out.

Could you please send me 4 bottles and I will give one back to Winooski?

Thanks,

JAck

Officer Jack Lehneman
Colchester Police Department
Dispatch: 802-264-5555
Fax: 802-264-5561
jack.lehneman@colchesterpdvt.org

******NOTE NEW E-MAIL ADDRESS******

**"ONLY TWO DEFINING FORCES EVER OFFERED TO GIVE THEIR LIFE FOR YOU;
JESUS CHRIST AND THE AMERICAN SOLDIER"**

**"ONE DIED FOR YOUR SOUL;
THE OTHER FOR YOUR FREEDOM"**



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMaster DMT: 100157
 Location: Colchester PD
 Certification Date: 02/08/2012
 Installation Date: 09/12/2012


Date: 11/02/2015
 Time: 21:09:54

SUBJECT NAME:
 TEST TEST
 DOB: 11/02/1915 AGE: 100
 GENDER: M
 LICENSE #: 1234567 VT

TEST OPERATOR NAME:
 CHRISTOPHER M JONES
 AGENCY: COLCHESTER PD

BLANK TEST	0.000	21:10
CALIBRATION CHECK	PASSED	21:10
SIMULATOR VAPOR 34.0°C	0.097	21:11
SUBJECT SAMPLE (Vol=3.2L)	0.000	21:12
BLANK TEST	0.000	21:13

All alcohol values reported in g/210L
 Sim. Vapor Concentration 0.099
 Sim. Vapor Range 0.094 - 0.104
 Lot #: 15-12-100

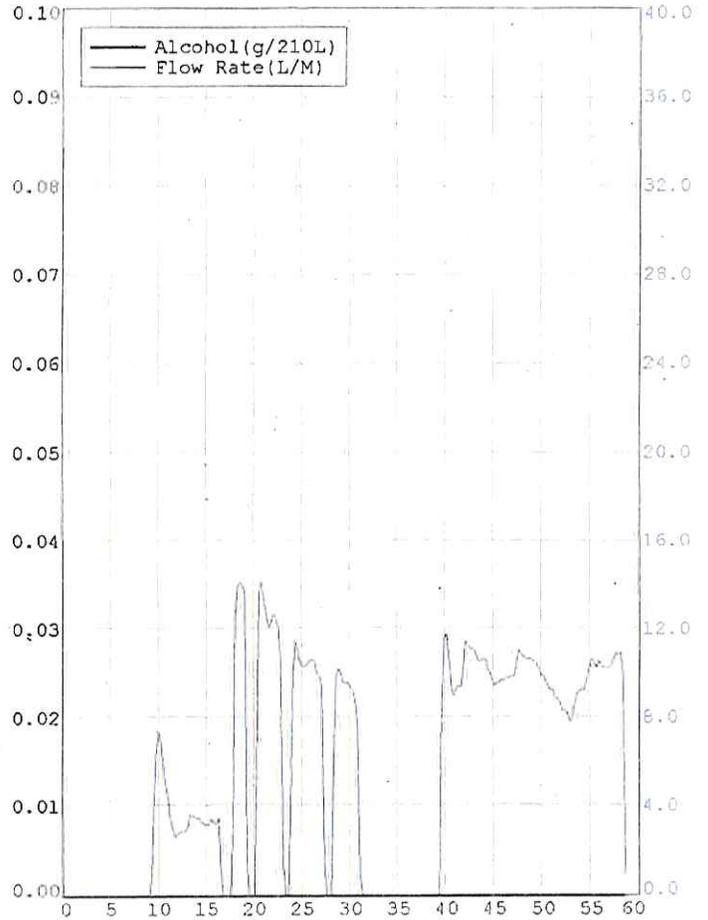

464 R9