DataMaster DMT Monthly Update Check-list

Department/Agency: MILTON P.D. DM serial #: 100159

Supervisor: LAFOUNTAIN Date: 04/24/15

	Provided	None this month
Operators Logbook	☑	☐
Maintenance Logbook	☑	☐
Breath Test History Report	☑	☐
Status History Report	☑	☐
Log On History Report	☑	☐
Calibration Report	☐	☑
Certification Report	☐	☑
Installation Report	☐	☑
Annual Preventative Maintenance	☐	☑
Routine Performance Check	☑	☐
Simulator Solution Change	☐	☑
Other Reports	☐	☑

List other report type and date:

ALL DATA INCLUDED FROM 01/01/15 - 04/24/15

DATAMASTER DMT OPERATOR USE LOG

Department/Agency

DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
08/19/14	SCALISE	MANDY BUSTER	.097	
10/27/14	Hendry	Wayne Snyder	.098	.096
10/29/14	Larente	TEST/RPC	.097	
11/19/14	LAFOUNTAIN	STEVEN MICA	.097	.095
11/22/14	Larente	Jacob Birdsall	.097	
11/29/14	Hendry	Brett Wallace	.097	
12/8/14	R. Driscoll	TEST / APM	.097	—
12/17/14	Hendry	Adam Provost	.094	
10/8/14	(TEST) LARENTE	TEST	.098	
2/22/15	Hendry	Jeremy Gay	.097	
2/24/15	LARENTE	TEST/RPC	.098	
2/28/15	Larente	Alfred Provost	.098	
3-24-15	Centabar	Goudette, Michael	.098	
4-12-15	Cooper	Nicholas Barella	.130	
04/21/15	COSTELLA	Mark D. CASTRO	.097	.097

ALC 603 Rev 3 08/11

DATAMASTER DMT MAINTENANCE LOG

Milton PD
Department/Agency

10059
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
12/8/14	Completed APM Protocol [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll DMT TECH
2/24/15	[For RPC or Simulator Solution Change Place Label Here] **DataMaster Simulator Solution** Lot # 14-14-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 10/16/2014 Expires: 10/16/2015 OPENED: 2-24-15 Larente RPC PASSED	Larente DMT Supervisor
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
01/17/2015	20:39:57	MILTON PD	JONATHAN E COOPER	0.135	0.126	0.094	0.095	
02/22/2015	21:13:58	MILTON PD	NICHOLAS J HENDRY	0.137		0.094		
02/28/2015	23:47:03	MILTON PD	EDOUARD A LARENTE	0.187		0.098		
03/24/2015	14:45:37	milton	JON G CENTABAR	REFUSED		0.098		
04/12/2015	05:17:51	MILTON PD	NICHOLIS M BARELLA	0.130		0.097		
04/21/2015	11:27:16	CHITTENDEN COUNTY SO	SCOTT COSTELLA	0.018	0.017	0.097	0.097	

Status Record History

Status Date	Status Time	Test Type	Status Message

Log On Record History

Test Date	Test Time	Name

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100159
Location: Milton PD
Calibration Date: 12/14/2011
Certification Date: 12/14/2011
Installation Date: 12/20/2011
RPC Date: 02/24/2015
Supervisor Name: ED A LARENTE

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 47.9°C
Digital Sim = 34.1°C

SETTINGS
Lamp Voltage = 1.81 V
Cooler Voltage = 1.83 V
Bias Voltage = 80 V
Chopper Freq = 537 Hz

PUMP INFO
Flow Rate = 5.758 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0421	0.0457
MIN(V)	0.0392	0.0439

FILTER INFO

Filter 1	0.044	Zero = true
Filter 2	0.286	Zero = true
Filter 3	0.556	Zero = true

CALIBRATION CHECK
Xq = 0.074 1.04%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-14-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

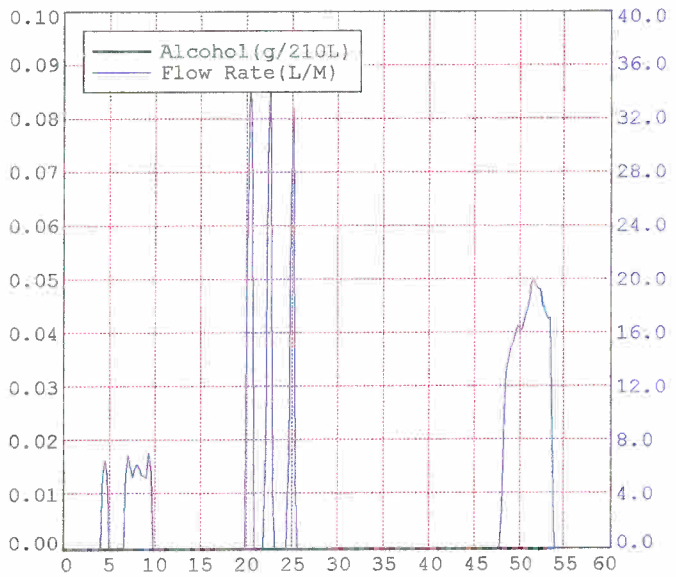

Performed by Ed A Larente Date 02/24/2015

Reviewed by _____ Date _____