INSTALLATION REPORT

DataMaster DMT: 100161
Location: Brattleboro VSP
Calibration Date: 08/22/2011
Certification Date: 08/22/2011
Installation Date: 09/02/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.79 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 532 Hz

PUMP INFO
Flow Rate = 5.537 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0205    0.0224
MIN(V)   0.0189    0.0209

FILTER INFO
Filter 1   0.022   Zero = true
Filter 2   0.335   Zero = true
Filter 3   0.534   Zero = true

CALIBRATION CHECK
Xq  = 0.086  0.51%
```

Accuracy and Precision Check

Concentration = 0.101 g/210L
Lot # = 11-41-100
Range = 0.096 - 0.106
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

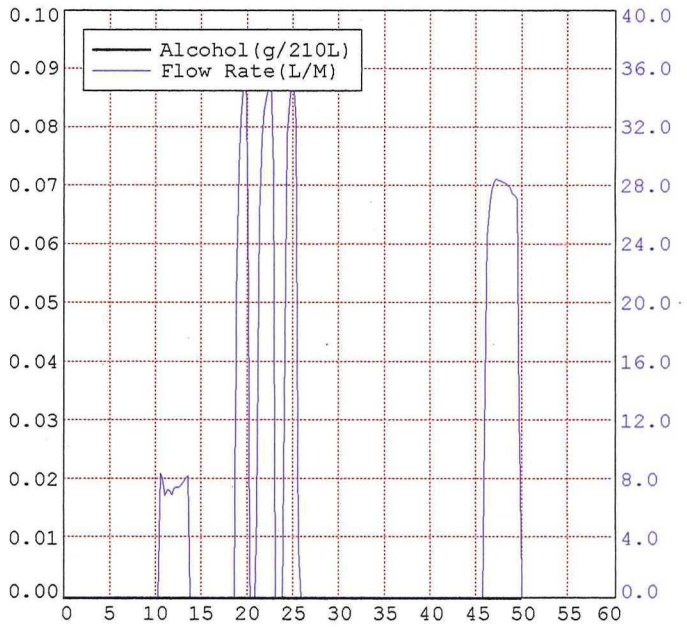

INSTALLATION PASSED

Performed by _____ Date 09/02/2011

Reviewed by _____ Date 9-2-11