ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100166
Location: Shaftsbury VSP
Calibration Date: 09/27/2011
Certification Date: 09/27/2011
Installation Date: 06/08/2012
RPC Date: 10/09/2013
Supervisor Name: JESSE W ROBSON

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube = 48.1°C
Digital Sim = 34.1°C

SETTINGS
Lamp Voltage = 1.74 V
Cooler Voltage = 1.70 V
Bias Voltage = 81 V
Chopper Freq = 562 Hz

PUMP INFO
Flow Rate = 6.216 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.1220	0.1262
MIN(V)	0.1203	0.1248

FILTER INFO
Filter 1 0.124 Zero = true
Filter 2 0.485 Zero = true
Filter 3 -0.087 Zero = true

CALIBRATION CHECK
Xq = 0.081 1.06%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration = 0.099 g/210L
Lot # = 13-04-100
Range = 0.094 - 0.104
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

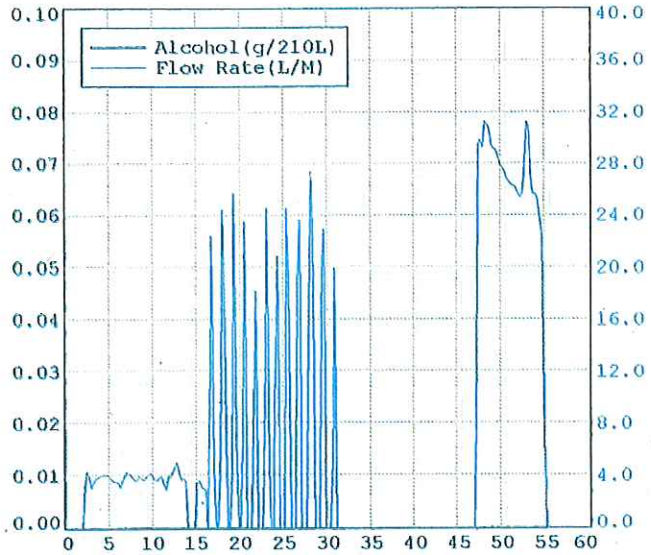

Performed by _____ Date 10/09/2013

Reviewed by _____ Date 10/10/13

10/10/2013