INSTALLATION REPORT

DataMaster DMT: 100169
Location: Bellows Falls PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/07/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.06
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.85 V
Cooler Voltage = 1.92 V
Bias Voltage   = 80 V
Chopper Freq   = 529 Hz

PUMP INFO
Flow Rate = 5.500 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.1002   -0.0982
MIN(V)   -0.1018   -0.0998

FILTER INFO
Filter 1  -0.099  Zero = true
Filter 2   0.241  Zero = true
Filter 3   0.530  Zero = true

CALIBRATION CHECK
Xq  = 0.095  0.18%
```

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 11-41-100
Range	= 0.096 - 0.106
Average	= 0.102 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

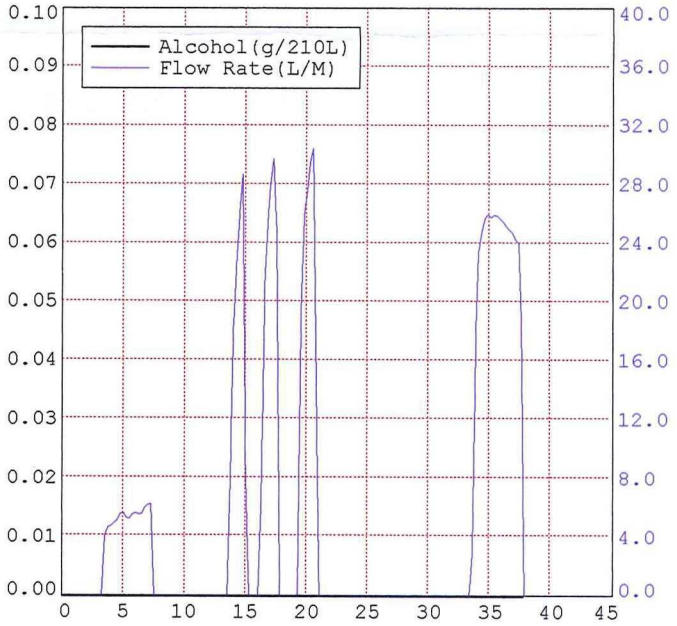

INSTALLATION PASSED

Performed by _____ Date 09/07/2011

Reviewed by _____ Date 09/07/11

Rev. [illegible] 9-8-11