ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100169
Location: Bellows Falls PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/07/2011
RPC Date: 02/01/2012
Supervisor Name: MICHAEL J KEEFE

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.85 V
Cooler Voltage = 1.92 V
Bias Voltage = 80 V
Chopper Freq = 533 Hz

PUMP INFO
Flow Rate = 5.361 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	-0.0638	-0.0612
MIN(V)	-0.0657	-0.0630

FILTER INFO

Filter 1	-0.062	Zero = true
Filter 2	0.266	Zero = true
Filter 3	0.555	Zero = true

CALIBRATION CHECK
Xq = 0.095 0.09%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-32-100
Range	= 0.095 - 0.105
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

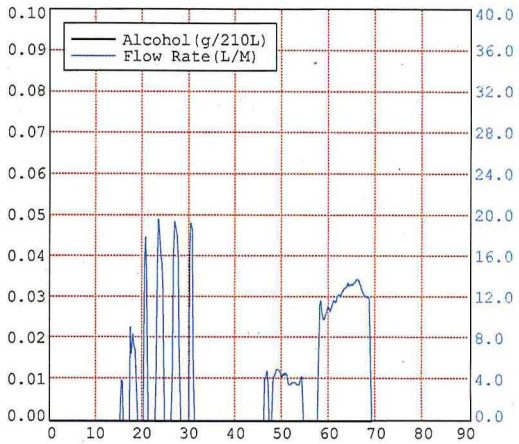

Performed by M. Keefe **Date** 02/01/2012

Reviewed by Steven Harnois **Date** 2/1/12

2/1/12

2-1-12

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
08/19/2011	11:23:30	VDHL	AMANDA BOLDUC	0.000		0.100		
08/19/2011	12:35:20	VDHL	AMANDA BOLDUC	0.000	0.000	0.100	0.101	
08/19/2011	12:55:56	vdhl	KIRK L KIMBALL	0.000		0.100		
08/22/2011	14:25:44	ADDISON COUNTY SO	YOUR FIRST YOUR LAST	REFUSED		0.100		
08/22/2011	14:48:13	ADDISON COUNTY SO	YOUR FIRST YOUR LAST	INCOMPLETE	REFUSED	0.100		
08/22/2011	15:12:12	ADDISON COUNTY SO	YOUR FIRST YOUR LAST	INTERFERENCE	0.097	0.100	0.100	
01/29/2012	02:23:35	BELLOWS FALLS PD	JED A MONTH			0.089		Simulator Out of Range
01/29/2012	02:27:33	BELLOWS FALLS PD	JED A MONTY			0.090		Simulator Out of Range
01/29/2012	02:34:37	BELLOWS FALLS PD	JED A MONTY			0.090		Simulator Out of Range