ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100169
Location: Bellows Falls PD
Calibration Date: 08/10/2011
Certification Date: 08/10/2011
Installation Date: 09/07/2011
RPC Date: 01/28/2015
Supervisor Name: MICHAEL J KEEFE

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 45.8°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.85 V
Cooler Voltage = 1.92 V
Bias Voltage   = 80 V
Chopper Freq   = 536 Hz

PUMP INFO
Flow Rate = 5.578 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2047    0.2069
MIN(V)   0.2035    0.2055

FILTER INFO
Filter 1   0.207  Zero = true
Filter 2   0.523  Zero = true
Filter 3   0.789  Zero = true

CALIBRATION CHECK
Xq  = 0.096  1.47%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.097 g/210L
Lot #	= 14-10-100
Range	= 0.092 - 0.102
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

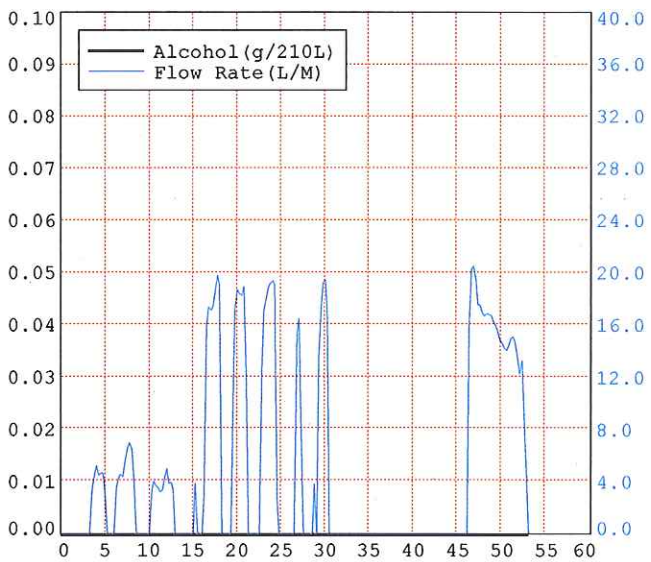

Performed by _____ **Date** 01/28/2015

Reviewed by _____ **Date** 1/29/15

1/29/2015