INSTALLATION REPORT

DataMaster DMT: 101708
Location: Royalton VSP
Calibration Date: 09/08/2011
Certification Date: 09/08/2011
Installation Date: 09/20/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.80 V
Cooler Voltage = 1.81 V
Bias Voltage   = 80 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 6.022 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0445    0.0457
MIN(V)   0.0429    0.0445

FILTER INFO
Filter 1   0.045  Zero = true
Filter 2   0.650  Zero = true
Filter 3   0.802  Zero = true

CALIBRATION CHECK
Xq  = 0.085  0.00%
```

Accuracy and Precision Check

Concentration = 0.101 g/210L
Lot # = 11-41-100
Range = 0.096 - 0.106
Average = 0.102 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

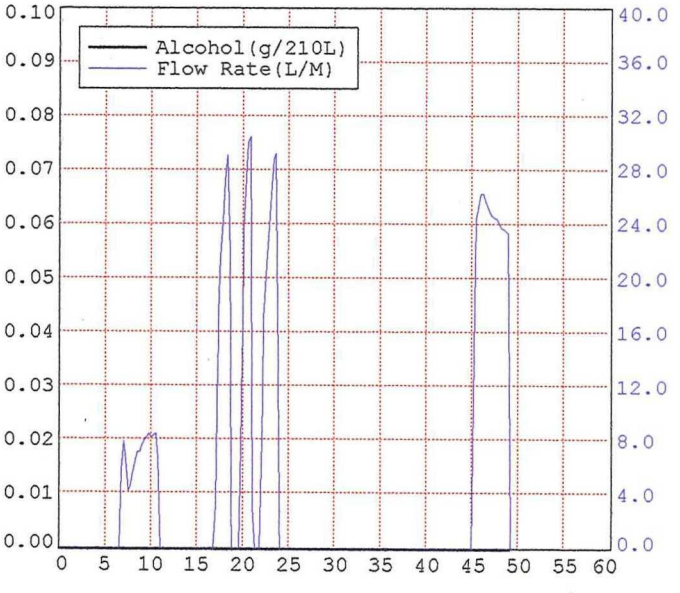

INSTALLATION PASSED

Reviewed 9/23/11 [illegible]

Performed by _____ Date 09/20/2011

Reviewed by _____ Date 9-20-11