ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 101708
Location: Royalton VSP
Calibration Date: 09/08/2011
Certification Date: 09/08/2011
Installation Date: 04/25/2013
RPC Date: 02/26/2016
Supervisor Name: STEVEN C STEARNS

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.80 V
Cooler Voltage = 1.81 V
Bias Voltage = 80 V
Chopper Freq = 543 Hz

PUMP INFO
Flow Rate = 5.985 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0600	0.0630
MIN(V)	0.0587	0.0614

FILTER INFO

Filter 1	0.061	Zero = true
Filter 2	0.667	Zero = true
Filter 3	0.801	Zero = true

CALIBRATION CHECK
Xq = 0.087 2.56%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 15-07-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0005

RF Detection Test

Passed

Sample Acceptance Test

Passed

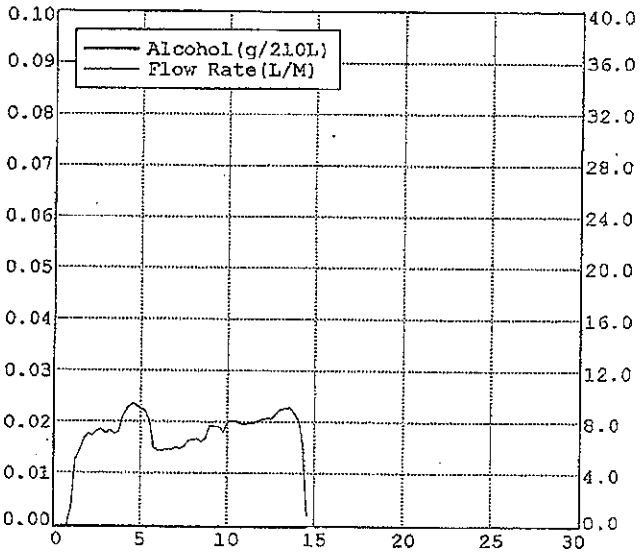

Performed by _____ Date 02/26/2016

Reviewed by _____ Date _____

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
03/19/2016	23:20:08	ROYALTON VSP	GARY T SALVATORE	0.100	0.100	0.095	0.095	
03/12/2016	03:13:01	ROYALTON VSP	MARK A BUSIER	0.192	0.199	0.096	0.096	
03/10/2016	01:29:58	ROYALTON VSP	JOSEPH E PREGENT	0.159		0.098		
02/29/2016	09:24:20	ROYALTON VSP	STEVEN C STEARNS	0.000		0.100		
02/20/2016	17:29:33	ROCKINGHAM VSP	KELSEY E KNAPP	REFUSED		0.096		
02/20/2016	01:09:17	ROYALTON VSP	JOSEPH E PREGENT	0.126	0.130	0.096	0.096	
01/30/2016	10:40:48	ROYALTON VSP	CHRISTOPHER J BLAIS	0.097		0.096		
01/30/2016	09:47:03	ROYALTON VSP	STEVEN CUTTITA	0.089		0.096		
01/20/2016	20:15:19	ROYALTON VSP	KELSEY E KNAPP	0.070	0.072	0.097	0.097	

DATAMASTER DMT MAINTENANCE LOG

VSP Royalton
Department/Agency

101708
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
4/3/15	Completed Annual PM [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll DMT Tech
6/17/15	**DataMaster Simulator Solution** Lot # 15-05-100 EtOHaq Conc: 0.099 g/210L Range: 0.094 - 0.104 g/210L Preparation Date: 2/19/2015 Expires: 2/19/2016 OPENED: 6/17/15 SS RPC - Sim Solution Change	Stearns
8/18/15	Downloaded data to USB drive, uploaded new [For RPC or Simulator Solution Change Place Label Here] Software, installed new Comm. PCB, and connected to DPS Network	R. Driscoll DMT Tech
10/30/15	**DataMaster Simulator Solution** Lot # 15-05-100 EtOHaq Conc: 0.099 g/210L Range: 0.094 - 0.104 g/210L Preparation Date: 2/19/2015 Expires: 2/19/2016 OPENED: 10/30/15 SS RPC & Sim Solution Change	Stearns
2/26/16	**DataMaster Simulator Solution** Lot # 15-07-100 EtOHaq Conc: 0.100g/210L Range: 0.095 - 0.105 Preparation Date: 5/11/2015 Expires: 5/11/2016 OPENED: 2/26/16 RPC & Sim Sol. Change	Stearns
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011

DATAMASTER DMT OPERATOR USE LOG

VSP Royalton
Department/Agency

101708
DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
11/21	Pregent	Spencer Brown	.098 .099	
12.9	ARCHAMBAU	DANIEL LARKIN	.099	
12/12	BUSIER	Charles Watters		
01/20	Knapp	William Pomeckau	.097	
01/30/16	CUTTITA	NATHAN MAYO	.099	
2/30/16	Pregent	Mathew Doyle	.096	.096
02/20/16	Knapp	Michael Kucka	.096	
2/26/16	Stearns	RPC & Sun Sil Chang	.100	
2/29/16	Stearns	TEST/RPC	—	
3/10/16	Pregent	Dustin R. McCloy	.098	
3/12/16	BUSIER	Michael Needham	.096	
3/19/16	SALVATORE	J. HELIE	.095	

ALC 603 Rev 3 08/11