INSTALLATION REPORT

DataMaster DMT: 102506
Location: Lamoille County SO
Calibration Date: 07/02/2013
Certification Date: 07/02/2013
Installation Date: 07/02/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube    = 47.3°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.78 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 533 Hz

PUMP INFO
Flow Rate = 5.396 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1797    0.1817
MIN(V)   0.1781    0.1803

FILTER INFO
Filter 1   0.182  Zero = true
Filter 2   0.757  Zero = true
Filter 3   1.559  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.73%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-04-100
Range	= 0.094 - 0.104
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

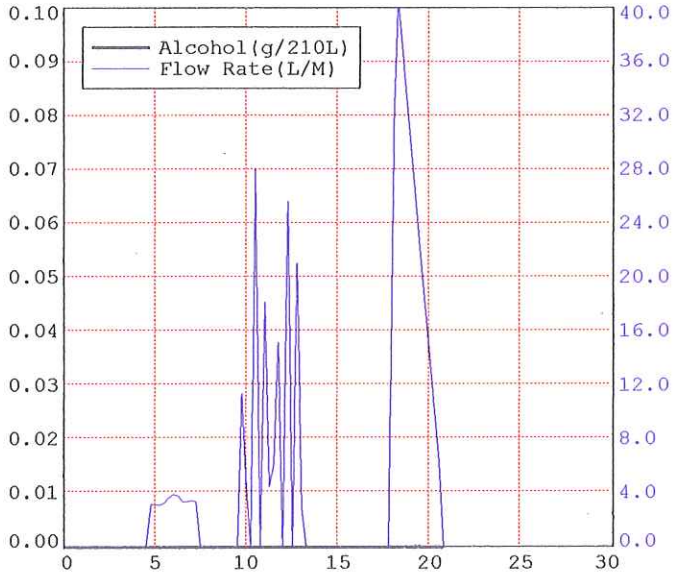

INSTALLATION PASSED

Performed by RCD **Date** 07/02/2013

Reviewed by **Date** 7/8/2013